



KAMIOKA GRAVITATIONAL WAVE TELESCOPE

JGW- T1200931-v1

*KAGRA*

26 March 2012

---

Transport features of the KAGRA type-B seismic  
attenuation chains and vacuum tanks.

---

Riccardo DeSalvo, Gianni Gennaro

Distribution of this document:

Public

This is an internal working note of the

***KAGRA* Large-scale Cryogenic Gravitational Wave Telescope Project.**

<http://gwcenter.icrr.u-tokyo.ac.jp/en//>

## 1 Introduction

Assembling and commissioning equipment inside the KAGRA [tunnels](#) has logistic difficulties, and result in a slower process. In addition the tight confines of the tunnel will limit the number of people working at any given time. Those people would be competing for the use of common instruments like the overhead cranes. In addition the KAGRA experimental halls will be ready rather late, any assembly and commissioning work that can be done externally will greatly accelerate the KAGRA commissioning. It is therefore important to do as much external pre-assembly and pre-commissioning as possible, store pre-assembled units as large and as complete as possible, ship them to the site as ready-to-fit units and limit the assembly in the tunnel to the minimum possible.

The safe transport of Virgo's payloads, with fused silica fibers, between Pisa and Roma, is the proof that complex structures, even much more delicate than the type-B towers, can be safely transported without damage or loss of accuracy.

KAGRA's type-B towers are described in and the [Type-B design](#) the [design philosophy](#), and [3D images](#) are available.

The type-B SAS seismic chains and payload have been designed and will be fully [assembled](#), [cabled](#), balanced, tuned and tested in a clean University laboratory. Unfortunately they are too large to be transported long distance in a single piece.

For road transport the KAGRA type-B seismic attenuation units have to be broken down in sections transportable on trucks.

Transport features have to be engineered into the system to allow safe transport from the assembly laboratory to the Kamioka mine. The transport must preserve the UHV cleanliness of the shipped sections, as well as all balancing and tuning pre-performed.

The SAS structures are too tall to fit on a truck, and need transport stiffeners to keep the suspended parts from hitting the safety structures and get damaged.

The SAS chain will be separated in two halves and transported from the laboratory to their final position in the KAGRA tunnels.

The following strategy has been devised.

## 2 Sectioning the SAS chain

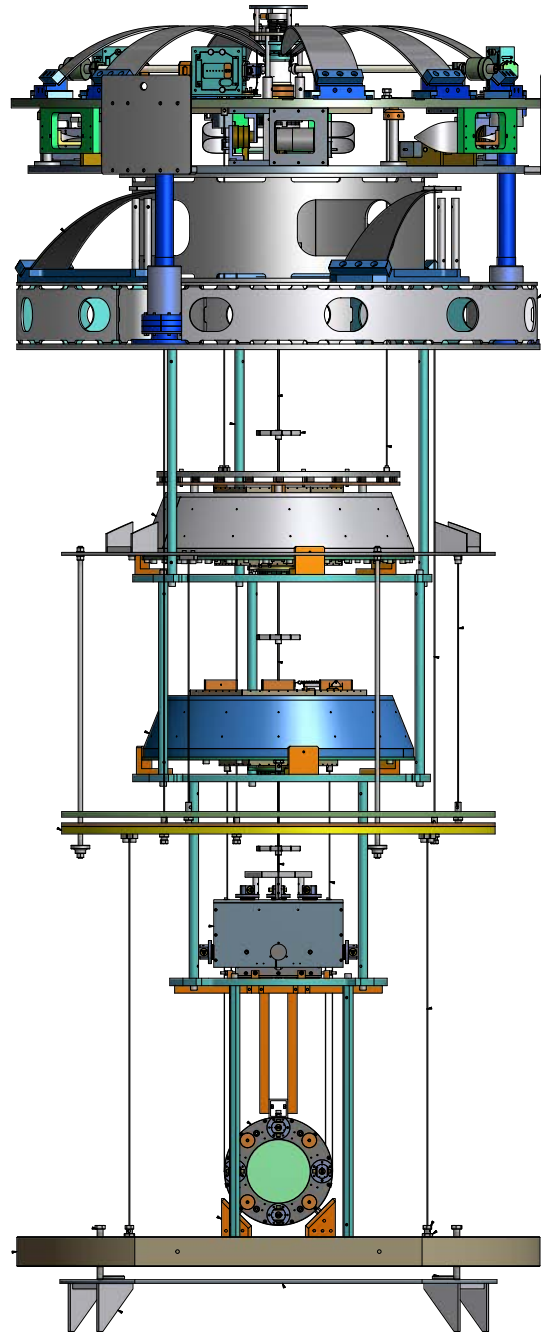


Figure 1: Type B chains and suspended optical bench (vacuum tank not shown)

The type B chains can be seen as composed by two parts, from now on called the seismic attenuator and its payload, and by the suspended optical bench. Note that this division is purely for convenience, the type-B seismic chains are an integrated structure with seismic attenuation and control functions distributed along the entire chain, and there is no physical division between the two arbitrarily separated halves.

As already discussed in the [assembly](#) report, the type B Seismic attenuator and its payload will be integrated in a single unit in a clean booth in the experimental hall. This unit can be lifted via crane from the clean booth and lowered directly into its vacuum tank, from above, with the optical bench already in place in the vacuum tank.

For long distance transport on a truck this unit will be further divided; the seismic isolator will be sectioned from its payload.

The optical bench illustrated in figure 2, the seismic attenuation, illustrated in figure 3 and the payload, figure 4 will travel separately.

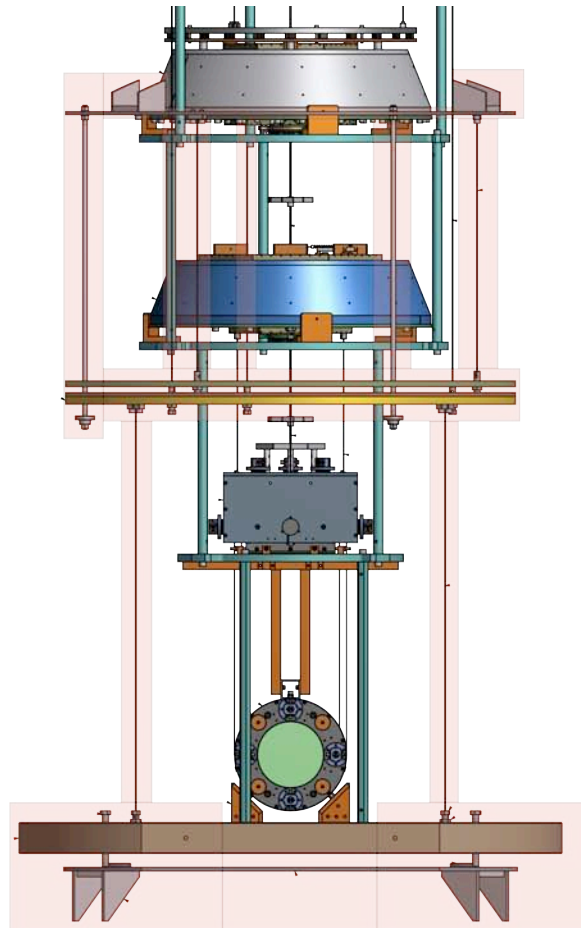


Figure 2: The structure of the optical bench is shaded in pink. The shelves above and below are welded to the inner surface of the tank. The optical bench, which will be fixed to its vacuum tank, will be mounted directly in loco.

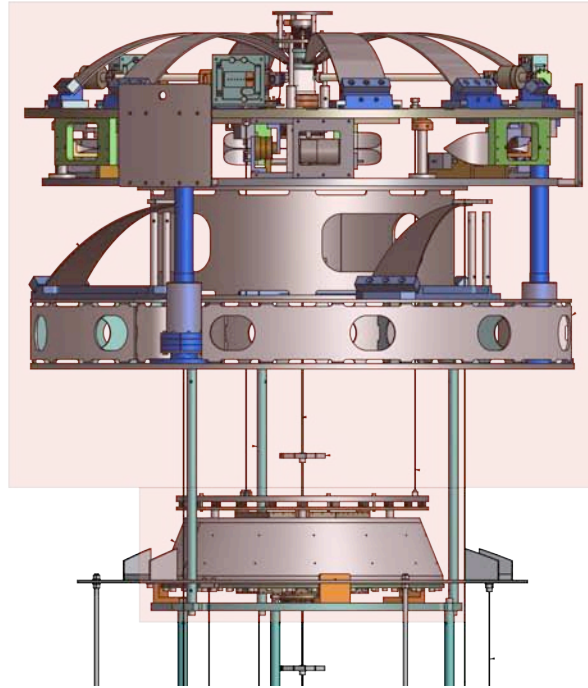


Figure 3: Seismic attenuation, composed of the pre-isolator, the standard filter, the Eddy current damper and the top part of the safety structure.

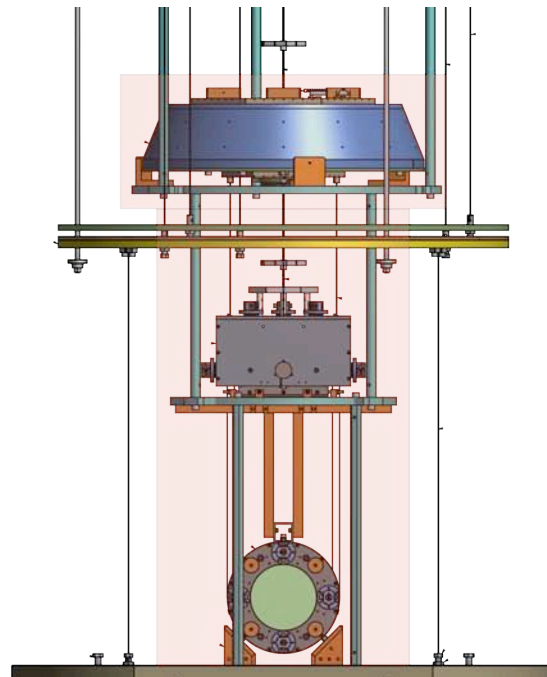


Figure 4: Payload, composed by the bottom filter, the intermediate mass and its recoil mass, the mirror and its recoil mass, and the lower section of the safety structure.

Only a limited amount of parts have to be removed in preparation for shipment:

- the suspension wire between the standard filter and the bottom filter
- the electrical cabling between the standard filter
- the three tie rods, between the upper and lower sections of the safety structure
- the three wires supporting the intermediate mass of the suspended optical bench.

The parts to be removed (except the electrical ribbons, which are not shown) are illustrated in figure 5.

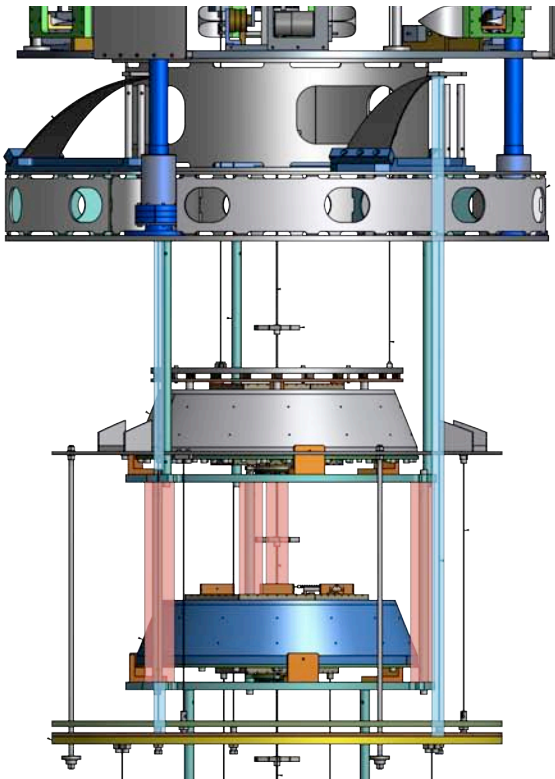


Figure 5: Components to be removed to section the seismic isolation from the payload. Shaded in pink are the mirror suspension wire and the four tie rods connecting the upper and lower section of the earthquake safety structure. Shaded in light blue are the three suspension wires of the optical bench intermediate mass.

The three wires connecting the pre-isolator to the optical bench intermediate mass would be anyhow mounted separately, after the entire seismic attenuation chain is lowered into the vacuum tank.

The electrical cabling for controls, running along the chain, are not shown in figure 5. To disconnect the wiring a crown of male sub-D connectors are mounted on the side of the bottom filter as illustrated in figure 6.

The disconnected cables, with their female connectors will be unclipped from the hexagonal cable rack on the top of the bottom filter, unclipped from the cabling spider along the suspension wire, rolled up, and temporarily secured to the hexagonal cable rack on the bottom of the standard filter.

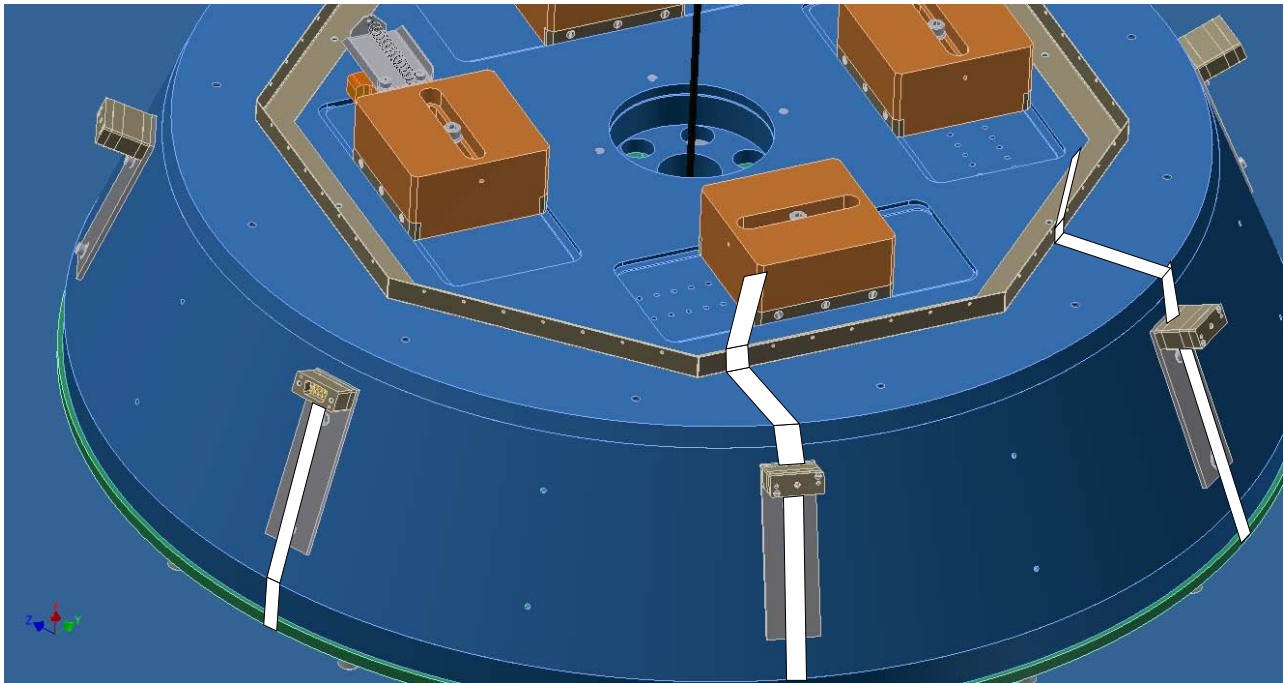


Figure 6: Crown of [connectors](#) mounted on the bottom filter. The ribbon cables coming from below end in the male connectors bolted to the lateral surface of the bottom filter. The cables coming from above are clipped to the octagonal shelf, and then fold up towards the cabling spider above. To separate the two halves of the chain, the cables are disconnected, unclipped from the shelf, and from the spider, and rolled up all the way to the standard filter above.

## 2.1 Immobilizing all components for shipment

Even after being disconnected the seismic isolator and the payload cannot safely travel without many, small precautions, to immobilize all moving parts and keep them from bouncing around and being damaged.

Special travel containers, very rigid and almost water tight, will keep the sections clean and safe during transport.

At the end of the transport the two sections will be re-united in a clean booth and rapidly inserted in the vacuum chamber.

The rest of the report discusses the details of immobilization of all moving parts, and the travel containers.



## 2.2 The Top transport tank

The transport tank for upper half chain, shown in figure 7, weighs 395 kg, is about 1.5 m in diameter and 1.75 m in height.

The gross weight of the isolation chain (including only Type B pre-isolator and standard filter) is 1448 kg. The center of mass is xxx m from ground.

The tank has bottom ears for bolting to a transport pallet. A layer of soft expanded polystyrene is inserted between the tank and the pallet to reduce high frequency vibrations.

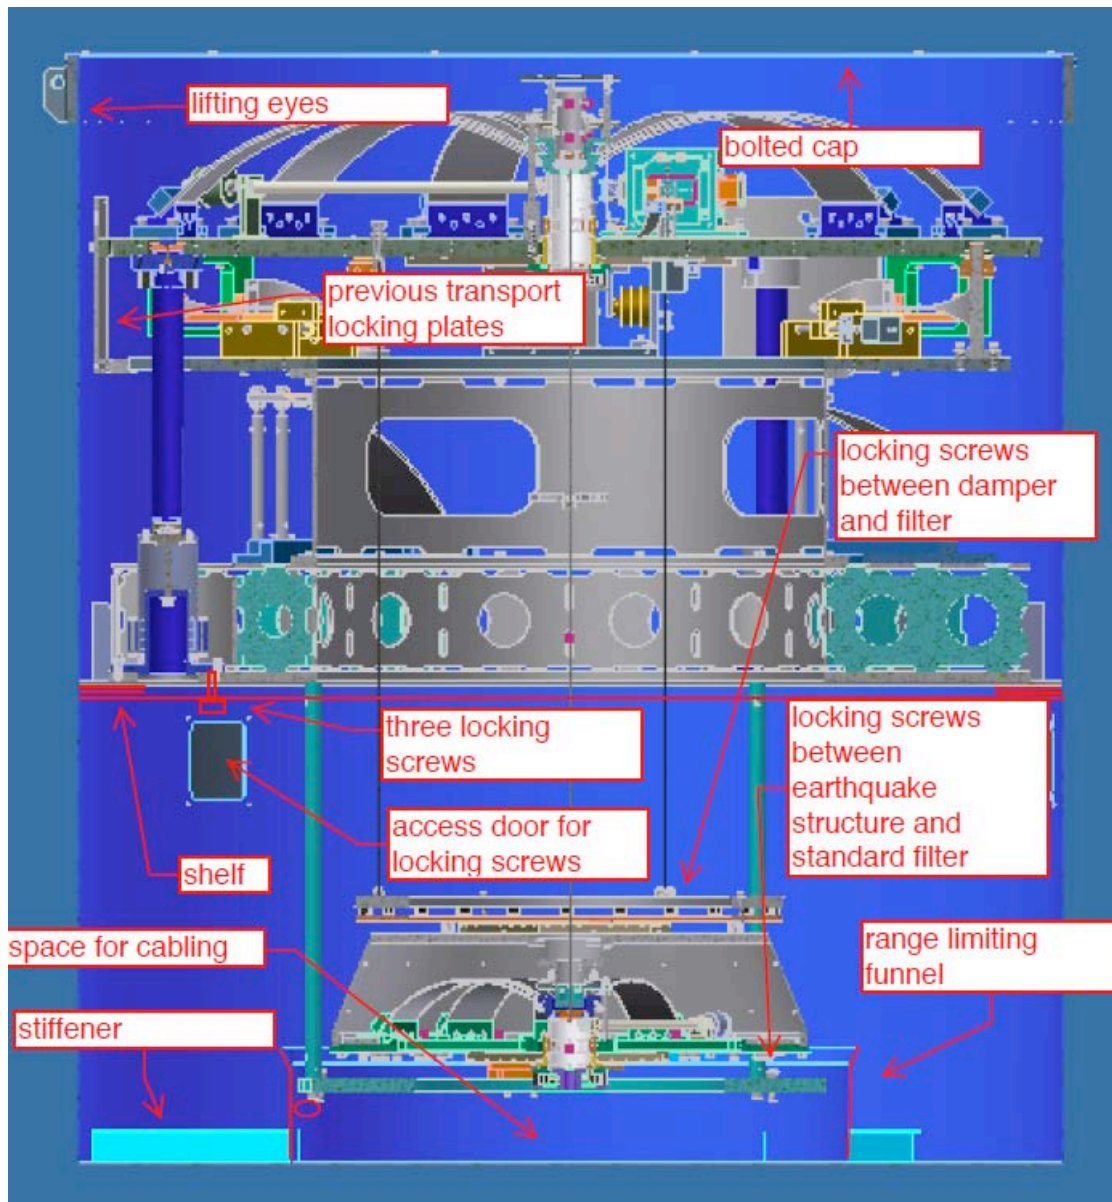


Figure 7: Transport tank loaded with the type-B seismic isolator.



The transport tank is a stainless steel tank with a shelf to support the pre-isolator base structure, stiffener that also act as insertion guides, and a cup at the bottom to immobilize the transversal motion of the safety structure of the standard filter. The shelf is provided with three slots needed to lock the pre-isolator base with three M12 bolts. Three access windows are foreseen below the shelf, in correspondence with the slots, to reach the bolts.

A solid stiffener is welded at the rim of the tank, with three lifting eyes. The stiffener is also provided with numerous threaded holes to secure the cap.

The cup at the bottom has a slanted rim to ease insertion, and is tall enough to leave 10 cm empty space for the coils of cables temporarily secured below the standard filter, and protected by a thin sheet metal transport plate.

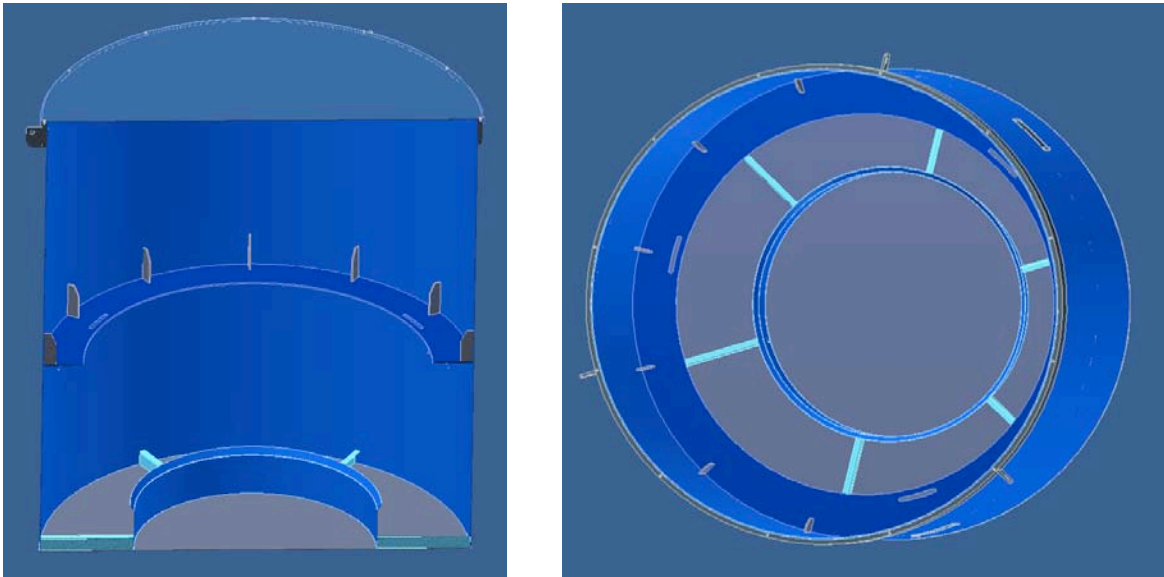


Figure 8: Cutout and top view of the tank.

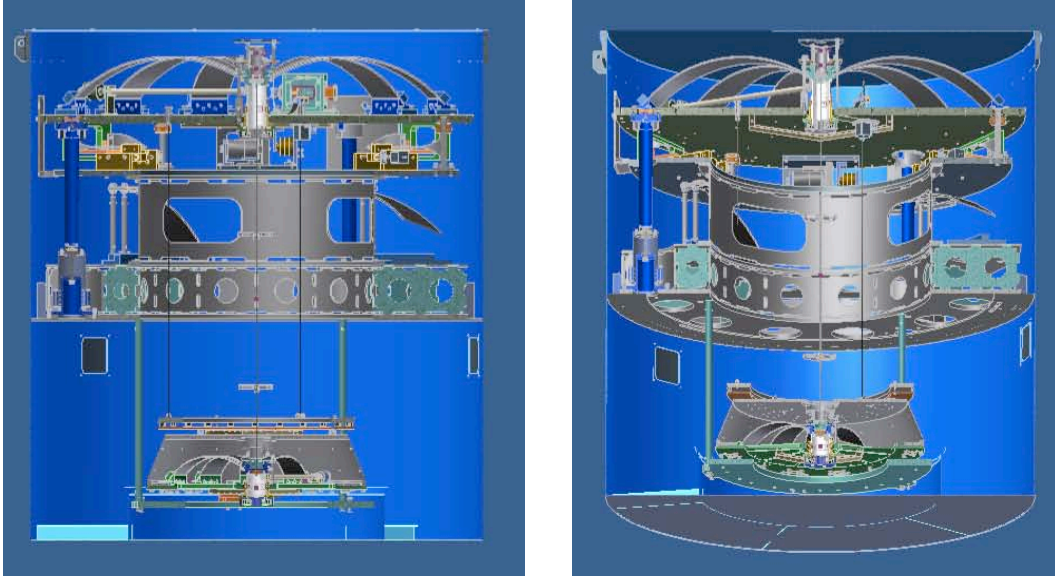


Figure 9: Side views of the loaded tank.

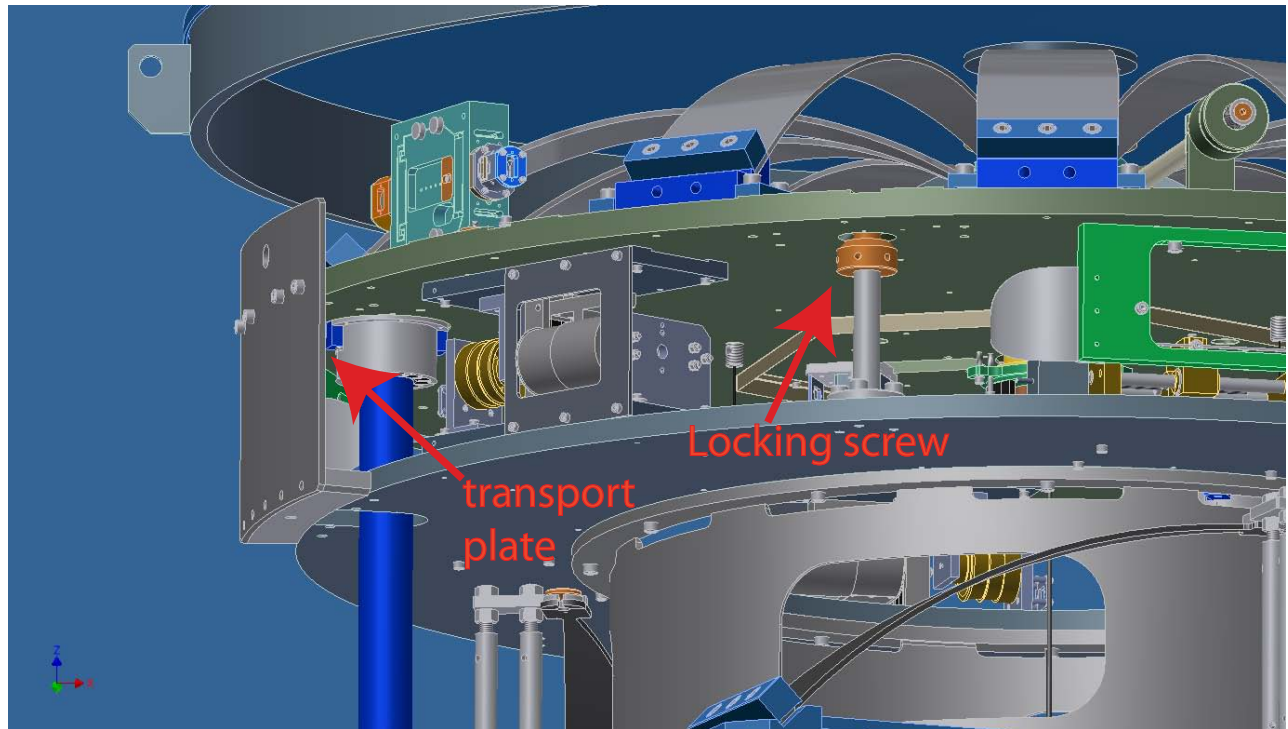


Figure 10 The orange screw-head are engaged to lock the horizontal movement of the IP. Then the transport plates are mounted to lock the Inverted pendulum to the base structure of the pre-isolator.

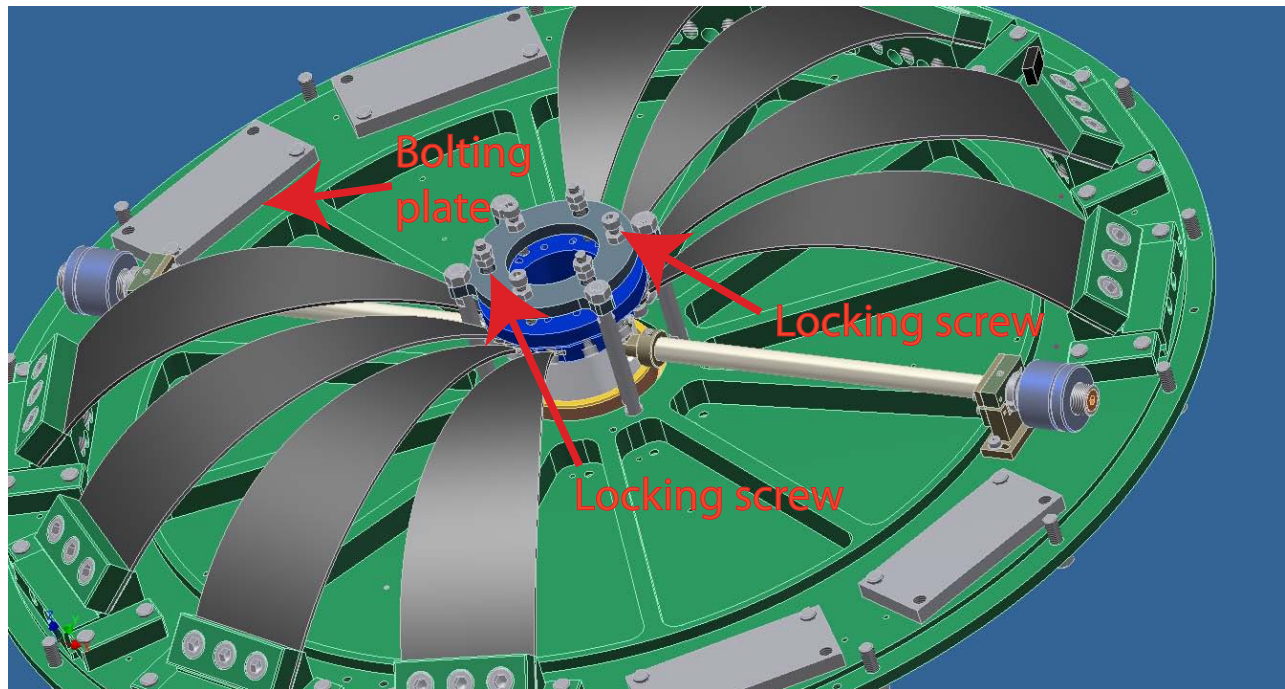


Figure 11: The three locking screws and nuts lock the vertical movement of the GAS springs. Bolting plates have been added in the empty slots of missing blades to provide threaded holes to lock the filter to its safety structure as illustrated in figure 12

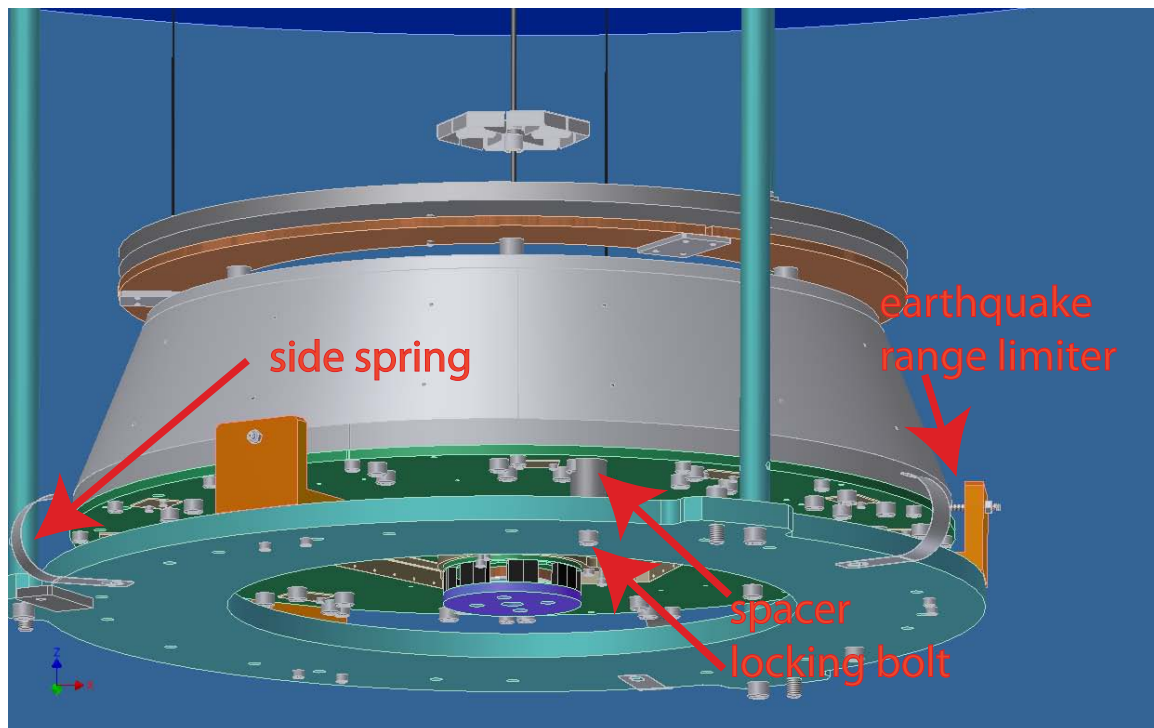


Figure12: The spacers and bolts lock the standard filter to its safety structure. The Earthquake range limiters can be engaged as well. The side spring mounted for transport hold the safety structure firmly inside the transport can

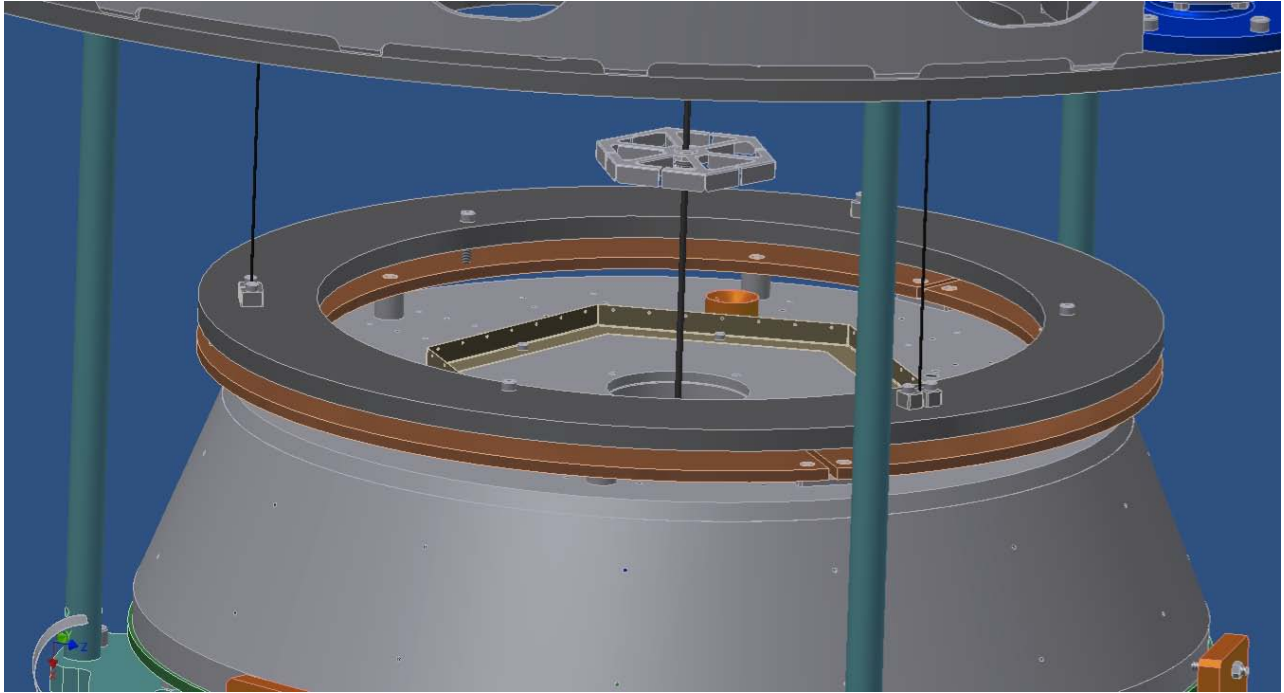


Figure13: Three bolts lock the magnetic damper ring to its copper ring on the top of the standard filter.

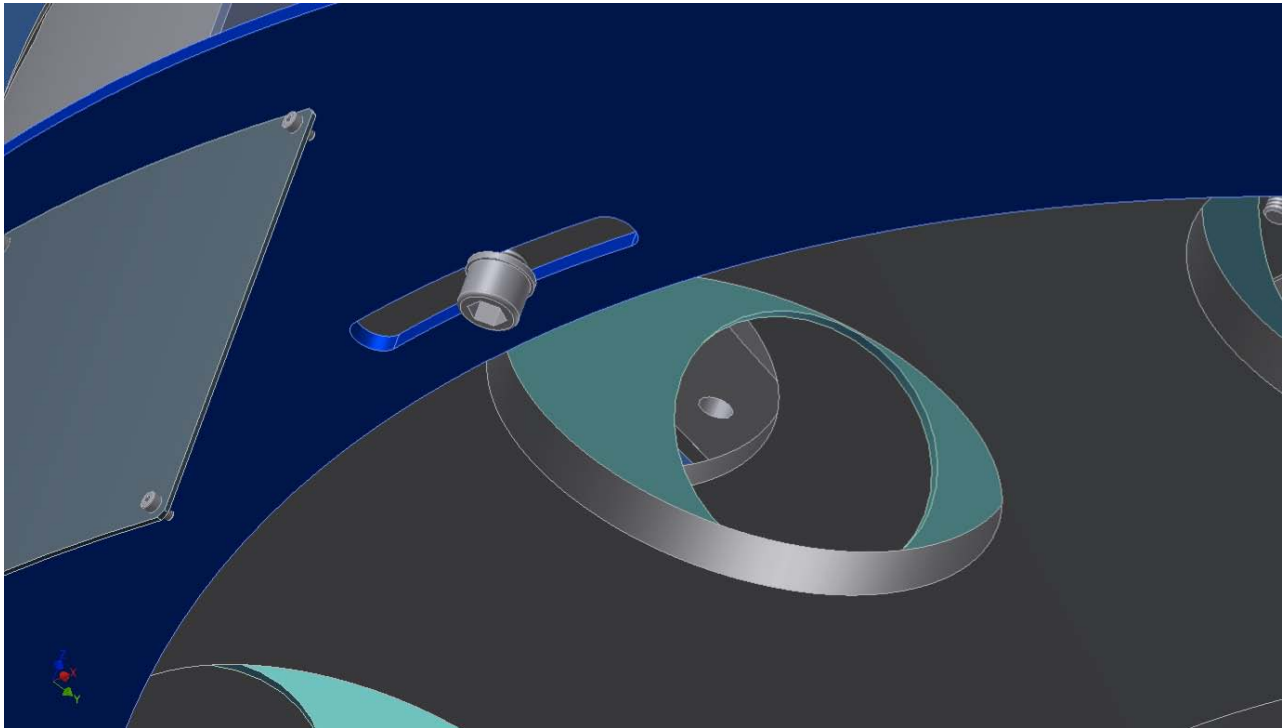


Figure 14: Three bolts secure the base of the pre-isolator to the transport tank.



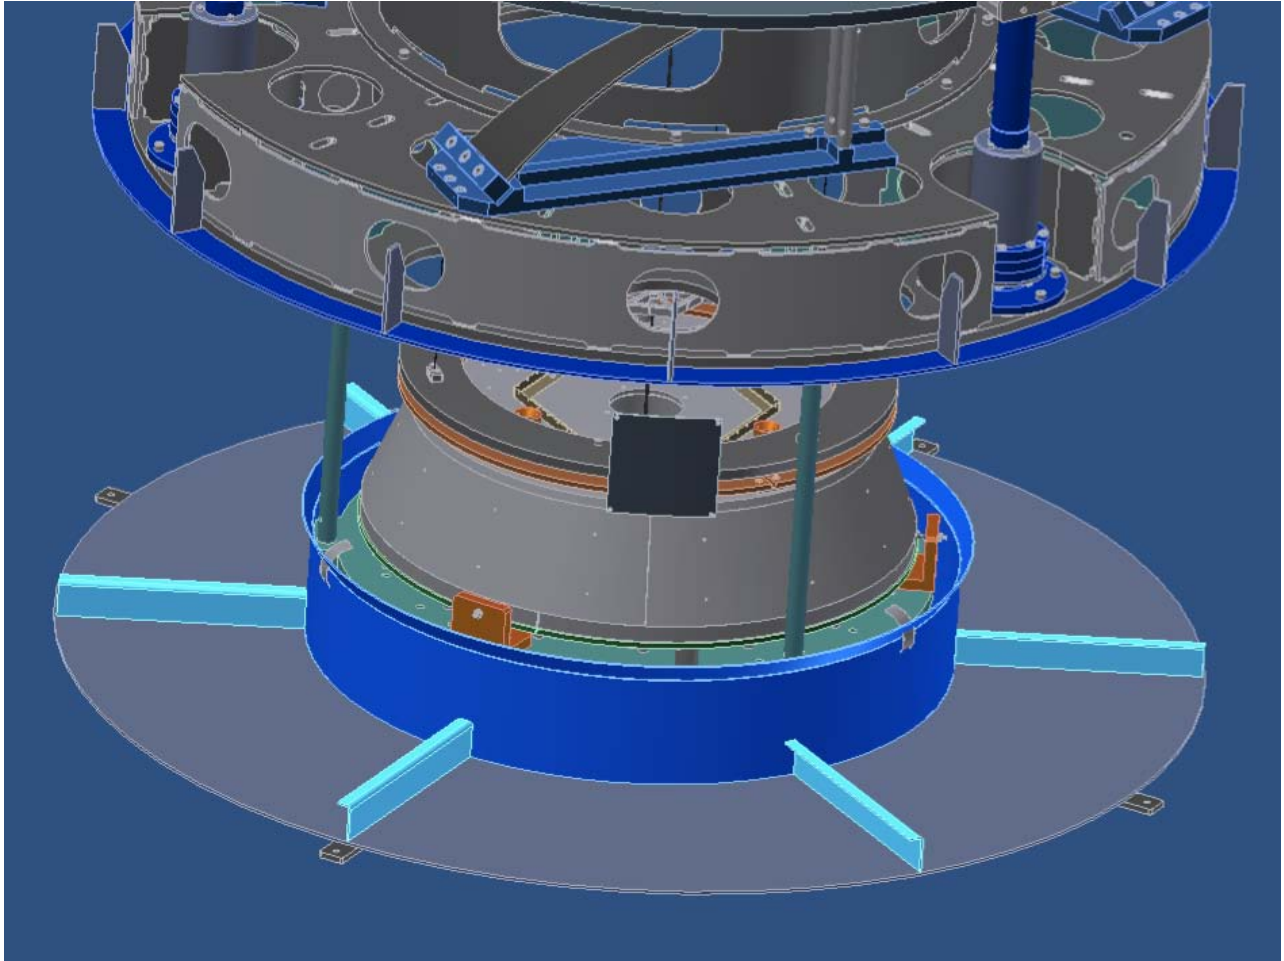


Figure 15: The safety structure fits inside the cup at the bottom of the tank, where the side springs shown in figure 12 impede the lateral oscillation of the standard filter against the safety structure.

### 2.3 The Bottom transport tank

The transport tank for the payload is smaller, but otherwise similar to the large tank.

The transport tank for the payload, shown in figure xxx, weighs xxx kg, is about xxx m in diameter and xxx m in height.

The gross weight of the payload (including its safety structure) is xxx kg. The center of mass is xxx m from ground.

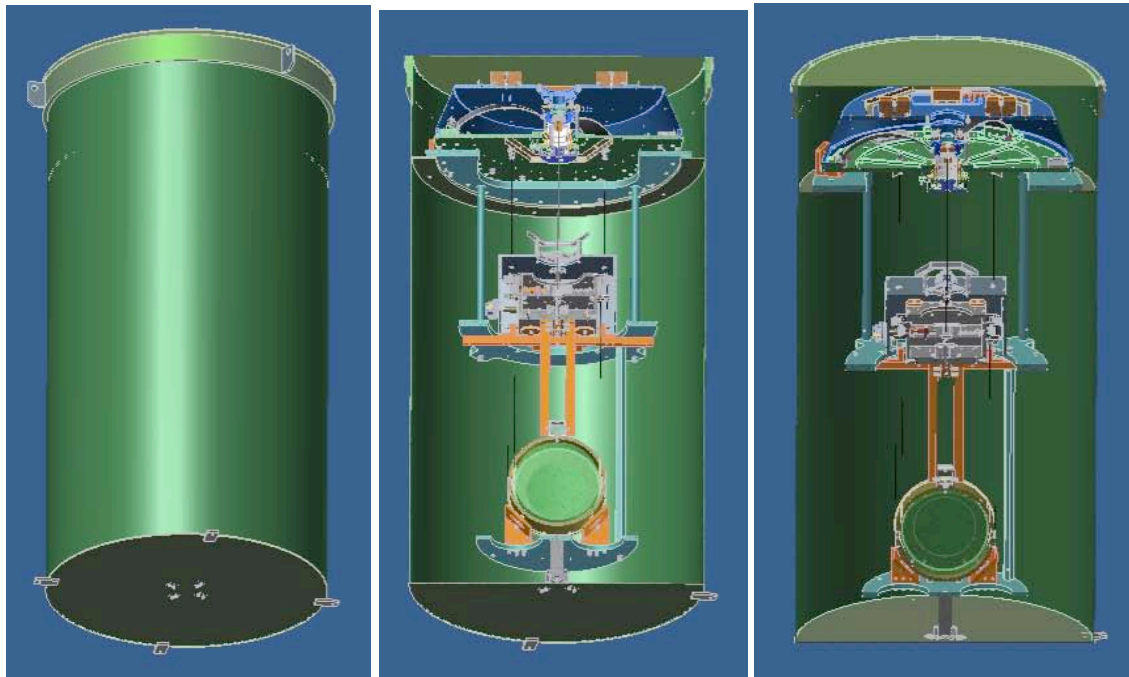


Figure 16: The transport tank for the payload is much smaller. The bottom plate of the tank is provided with bolting lips to attach the tank to a transport pallet. The payload locked into its safety structure is bolted from above onto a circular shelf.



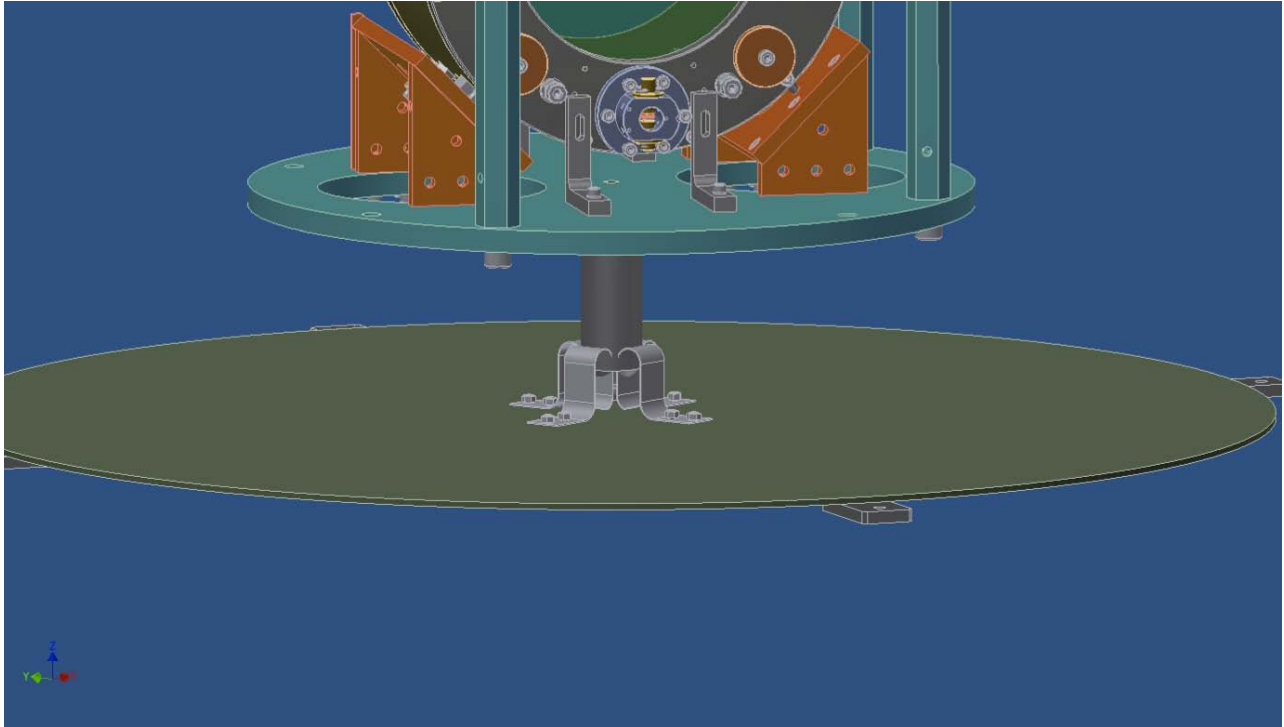


Figure 17: A temporary stud is screwed under the bottom of the payload safety structure. When the payload is inserted into its transport tank, the stud slips between 4 springs impeding its transversal motion.

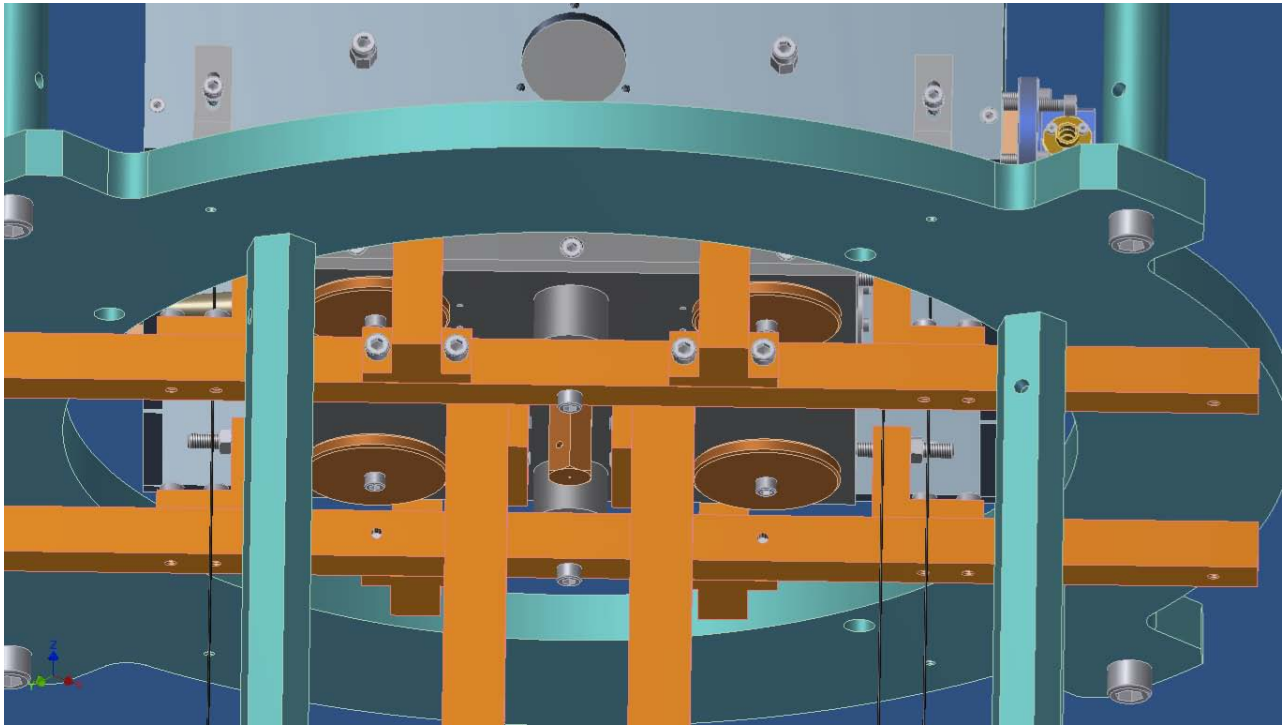


Figure18: Two bolts and spacers lock the intermediate mass to its safety structure.

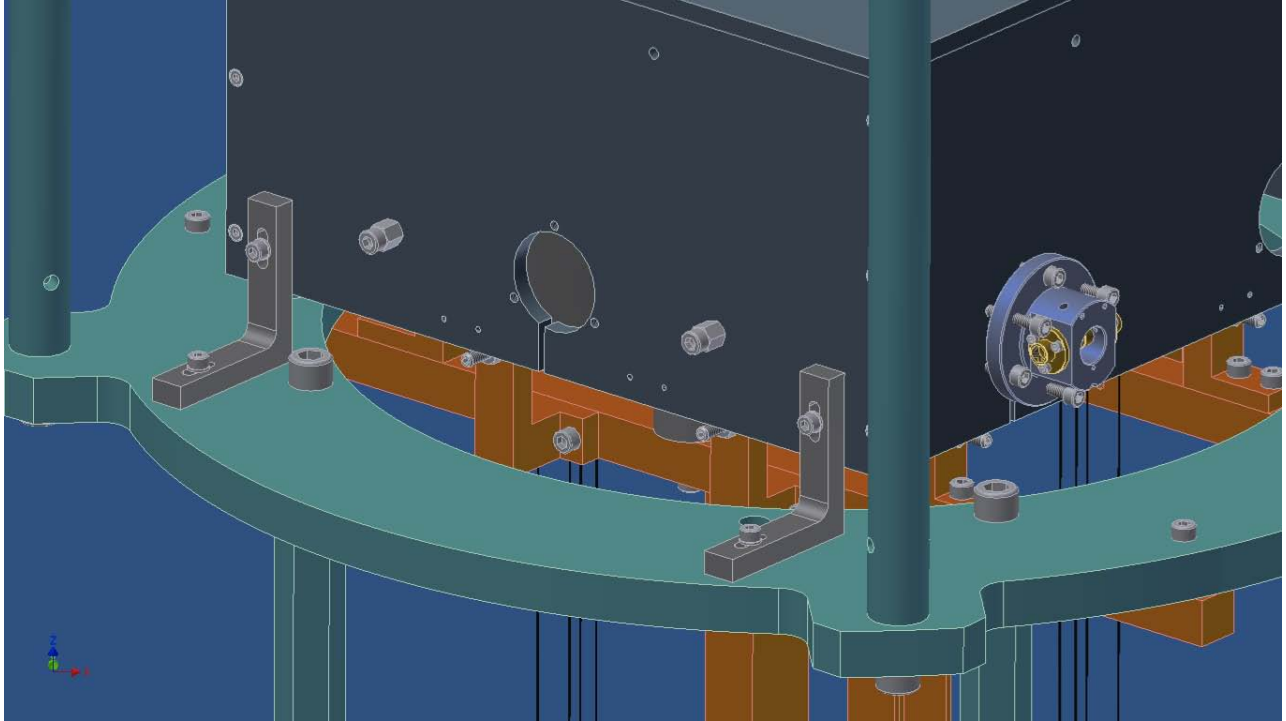


Figure19: Four brackets lock the transversal movement of the intermediate recoil mass. Note: slots are foreseen in the brackets because the intermediate mass and its recoil mass are first interlocked by tightening their mutual motion range limiting screws. The brackets are tightened down last.

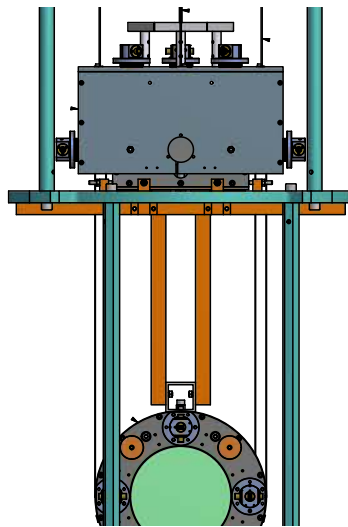


Figure 20: Two bars tie the intermediate mass to the mirror recoil mass.

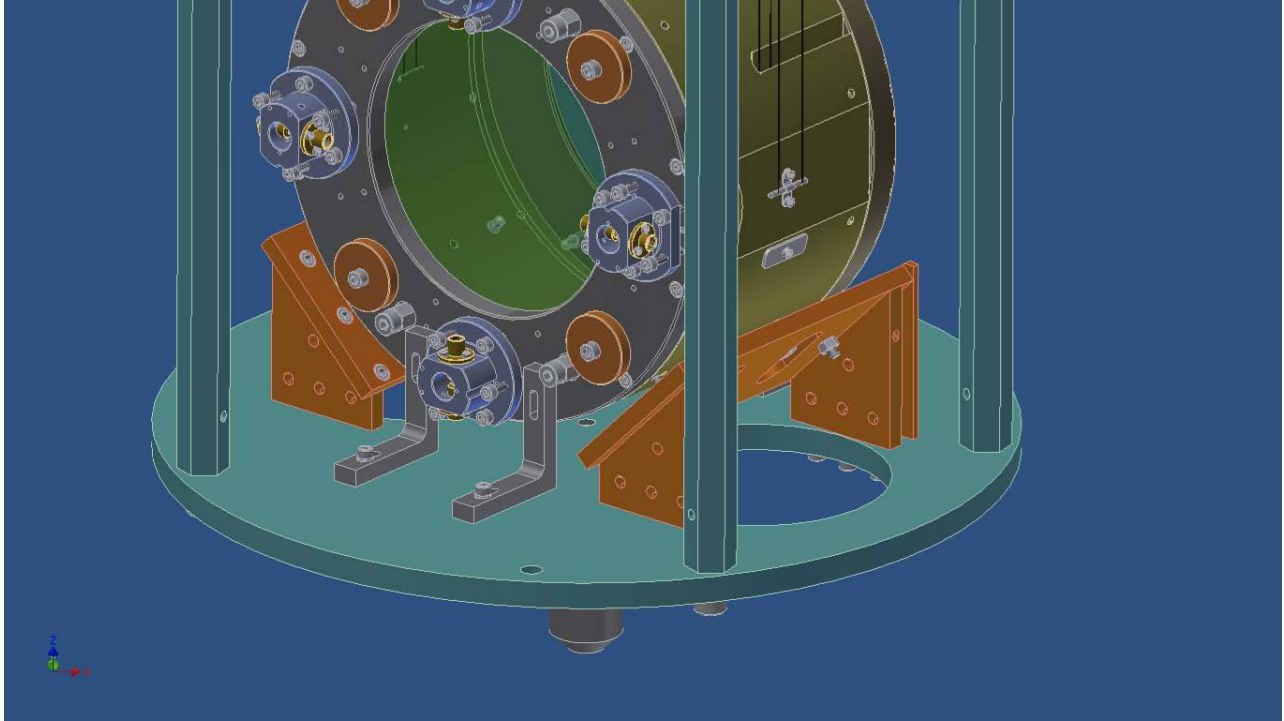


Figure 21: The mirror is locked inside its recoil mass by tightening its range limiting screws, after inserting Nylon spacers. Four brackets lock the longitudinal motion of the mirror recoil mass, they only sit against it, because the recoil mass is already solidly locked in the vertical direction.

### 3 The UHV vacuum tanks.

The vacuum tanks are delivered with protection flanges on the large ports and blind conflat flanges in all smaller ports. The tanks are rigid enough that they can be rotated 90° and safely travel on flat bed trucks. They can be lifted from the truck by the experimental hall crane, and raised back to their vertical position. Because they are sealed, the UHV cleanliness inside the tank is automatically preserved.

### 4 Moving the fully assembled and tuned Type-B SAS towers along the KAGRA tunnel.

There is an interesting option that can be considered.

The type-B SAS towers are designed for the beam splitter and recycler mirrors. Their SAS unit is designed to be assembled in a clean room inside the experimental hall, then lifted with the crane, and lowered in its vacuum chamber. This operation is adequate for its use in b-KAGRA.

There is an option that can be considered. In initial KAGRA will have no power recycling and no signal recycling, therefore only two of the three power recycler mirrors will be necessary to allow the beam to follow the dog-leg path leading to the beam splitter. Therefore four Type-B towers will be initially unused.

The type-B towers are designed to carry the same mirror size as the four main mirrors of i-KAGRA. Therefore there would be a great economical and manpower advantage, as well as an acceleration of the commissioning, if the four available Type-B towers could be used to suspend the i-KAGRA main mirrors.

#### 4.1 Aircushion transport

The main problem is that there is low ceiling and no crane to assemble the Type-B towers in the places of the ITM and ETM of iKAGRA.

There is a second problem that the few m of tunnel between the experimental halls and the i-KAGRA ITM and ETM are 4 m tall, 70 cm lower than the Type-B towers (figure 22). If these few meters of tunnel can be made 80 cm taller, the following scenario can be enacted.

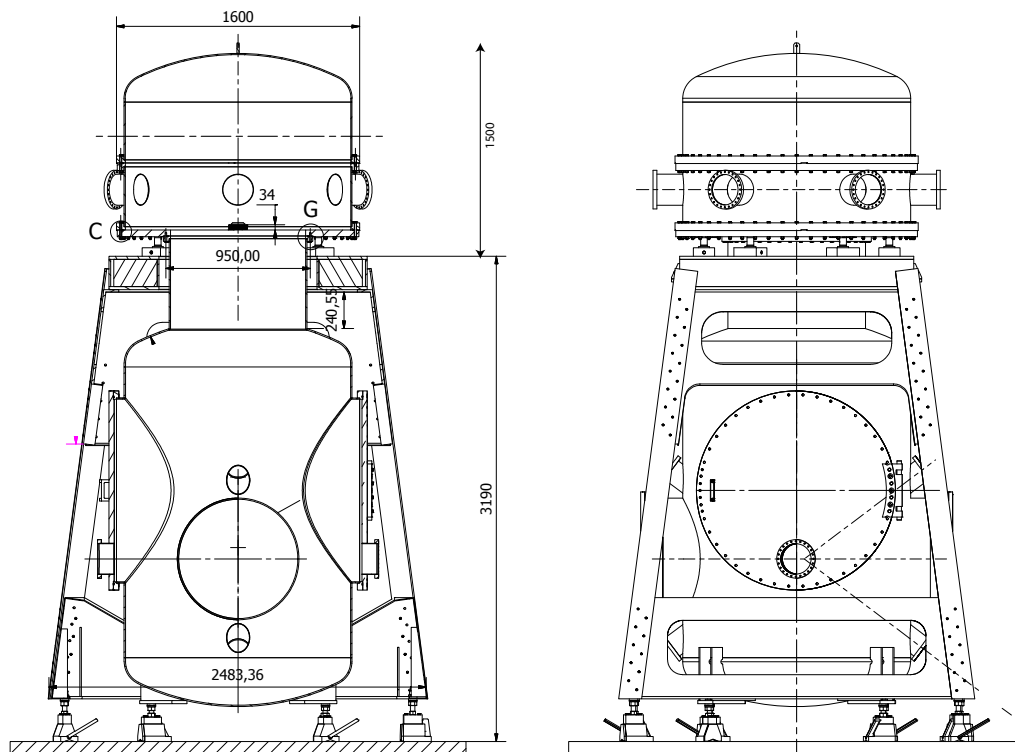


Figure 22: dimensions of the Type-B SAS towers.

The Type-B SAS towers can be fully assembled in the central or in the end experimental halls, and then transported fully functioning, already loaded with their mirrors, in the working location. This can be safely and precisely done with aircushion plates, an operation that is commonly done industrially, as can be seen in:

[http://www.youtube.com/watch?v=PEwDu8ka\\_RI](http://www.youtube.com/watch?v=PEwDu8ka_RI) and <http://www.aerofilmsystems.com/products>.

At CERN the 2,000 or 3,000 tons of the AU2 experiment were precisely moved in and out of the beamline by aircushion, propelled by a modified bicycle.

A much simple system can be implemented at i-KAGRA. A steel plate 2.5x2.5 m can be fitted with a 10 cm wide, bolted rim structure, with a rubberized cloth mounted as illustrated in figure 23.

The entire Type-B SAS structure, can be mounted on the plate, and magnetically clamped (it is already provided with magnetic clamps for relocation).

Air is blown inside the rubberized cloth pocket circling the plate, thus generating a soft seal to the ground. Properly located holes in the cloth pressurize the air below the plate. Less than 0.1 atmosphere pressure, provided by a blower, is sufficient to lift the tower. Then it can be pushed by hand.

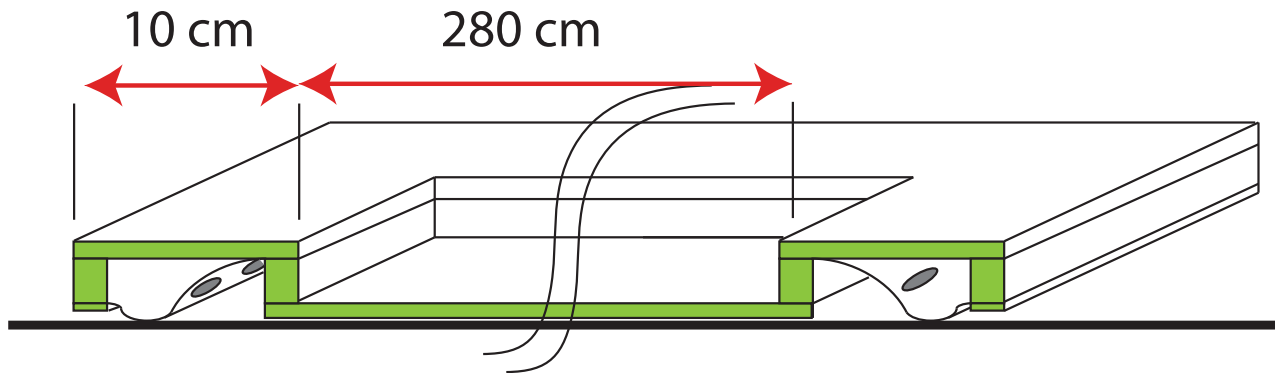


Figure 23: Schematized aircushion plate to move type-B SAS towers at KAGRA.

The Type-B SAS tower, complete of its vacuum tank and external structure, can then be drifted on the floor to the desired location, provided that the floor is sufficiently flat. Even steps can be passed with a “Panama” approach of shimmed plates.