

KAGRA Actuator Noise Modeling Report

Yuta Michimura

April 21, 2015

1 Introduction

This report is to summarize the results of actuator noise modeling for the KAGRA suspensions. The modeling was done by using MATLAB Simulink based NoiseBudget script made by Chris Wipf [1].

The main script and the model for the actuator noise modeling are as follows:

- https://granite.phys.s.u-tokyo.ac.jp/svn/LCGT/trunk/kagranoisebudget/Suspensions/run_SAS_NB.m
- <https://granite.phys.s.u-tokyo.ac.jp/svn/LCGT/trunk/kagranoisebudget/Suspensions/SAS.slx>

You will also need `findNbSVNroot.m`, `myzpk.m`, `plotdobe.m`, and `plotspectrum.m` in the same directory to run the script.

The main purpose of this modeling is to check if the actuator noise meet the displacement noise requirement set by MIF group, and to check if the feedback signals to the actuators does not saturate DACs. Small actuation efficiency gives less displacement noise, but it requires more feedback voltage.

Although this script works similarly for all suspensions, here I plot the results mainly for BS (Type-B suspension). Actuator design for ITM/ETMs is not fixed yet at this point.

2 Model

The Simulink model is shown together with the transfer functions and noises used for the simulation.

2.1 Simulink model

The actuator noise Simulink model is shown in Fig. 1. We had to use some tricks to simulate out-of-loop stability and feedback signal with Simulink NoiseBudget blocks, `NbNoiseCal` and `NbNoiseSink`. `FlexTf` is used for suspension transfer functions (light purple blocks) to use frequency response data (`frd`). Seismic noise from vertical coupling is also included in the model.

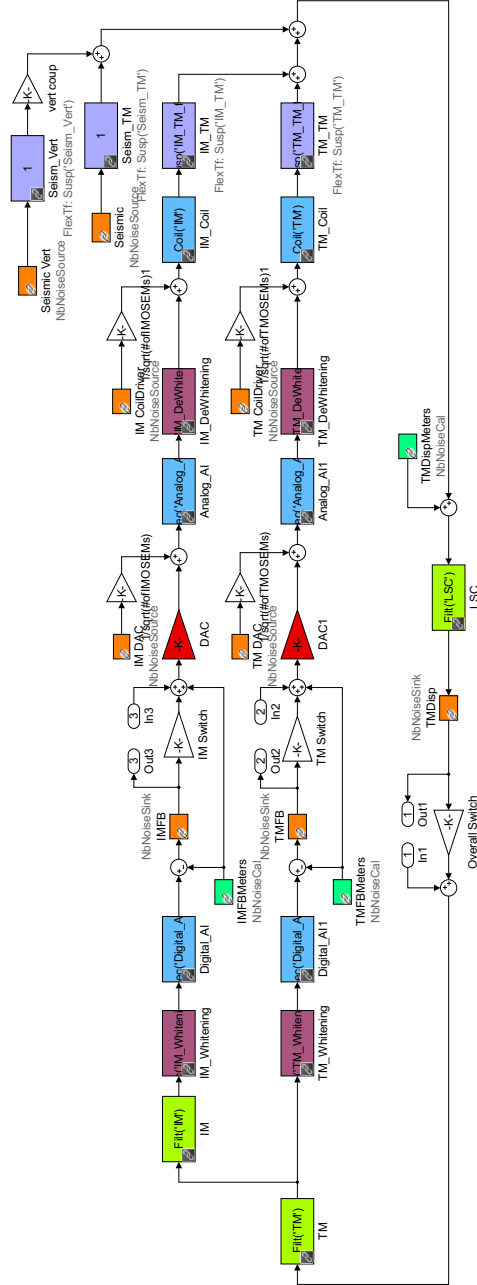


Figure 1: Actuator noise Simulink model.

2.2 Summary of KAGRA Suspensions

KAGRA suspension configurations are summarized graphically in Ref. [2]. For longitudinal degrees of freedom, we basically have actuators for IP (inverted pendulum), IM (intermediate mass), and TM (test mass).

Table 1 is the summary of the actuation for each suspension. Actuation efficiency for a Type-B/Bp coil in N/A is from Ref. [2]. Actuation efficiency for a Type-C TM coil are estimated from the measurement done by T. Saito [6]. The measurement for MCe gives 3.1×10^{-7} m/V at DC, and this gives 5.0×10^{-6} N/V assuming IMC mirror mass to be 0.47 kg and the resonant frequency to be 0.93 Hz. The V-I conversion of coil driver for IMC mirrors is 20 mA/V (50Ω), so this means the actuation efficiency for a Type-C TM coil is 6.3×10^{-5} N/A.

Table 1: KAGRA suspension actuator parameters. The TM/IM masses and wire lengths for Type-B/Bp suspensions come from Ref. [3]. Those for Type-A suspensions come from Ref. [4]. TM actuation efficiency for Type-C comes from Ref. [6].

Type	Type-A	Type-B (BS)	Type-B (SR)	Type-Bp	Type-C
Applicable mirrors	ITM,ETM	BS	SRM,SR2,SR3	PRM,PR2,PR3	MCi,MCo,MCE
Mirror diameter	$\phi = 220$ mm	$\phi = 370$ mm	$\phi = 250$ mm	$\phi = 250$ mm	$\phi = 95.95$ mm
Mirror thickness	150 mm	80 mm	100 mm	100 mm	29.5 mm
Mirror substrate	Sapphire	Fused Silica	Fused Silica	Fused Silica	Fused Silica
Mirror mass	22.7 kg	18.9 kg	10.8 kg	10.8 kg	0.47 kg
Intermediate Mass mass	53.2 kg	36.5 kg	15.6 kg	15.6 kg	1 kg?
Wire length between TM and IM	0.3 m	0.5 m	0.5 m	0.5 m	0.25 m
Wire length between IM and Platform/BF	0.4 m	0.5 m	0.5 m	0.5 m	0.25 m
TM actuation per coil [N/A]	??	0.129	0.129	0.129	6.3×10^{-5}
# of TM coils for long.	4	4	4	4	4
IM actuation per coil [N/A]	??	1.12	1.12	1.12	N.A.
# of IM coils for long.	??	1	1	1	0

2.3 Suspension transfer functions

The suspension transfer functions from actuation on IM/TM (from respective recoil masses) to TM displacement are shown below.

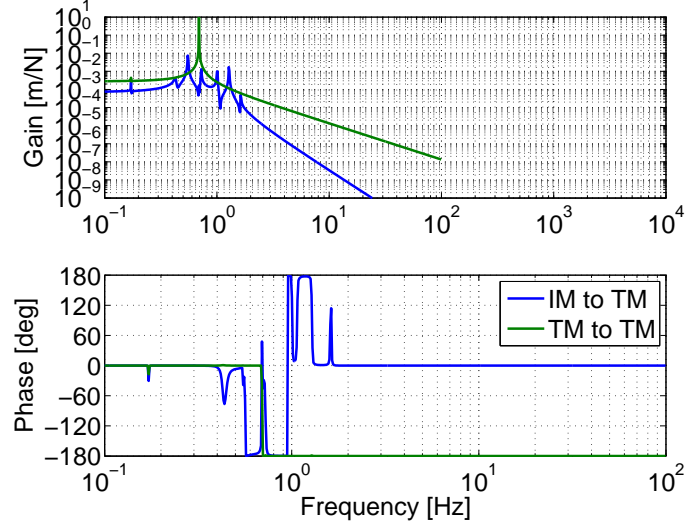


Figure 2: BS suspension transfer functions.

The seismic noise suppression ratio are shown below. The vertical one is also plotted. The vertical to longitudinal coupling was assumed to be 1% in the modeling.

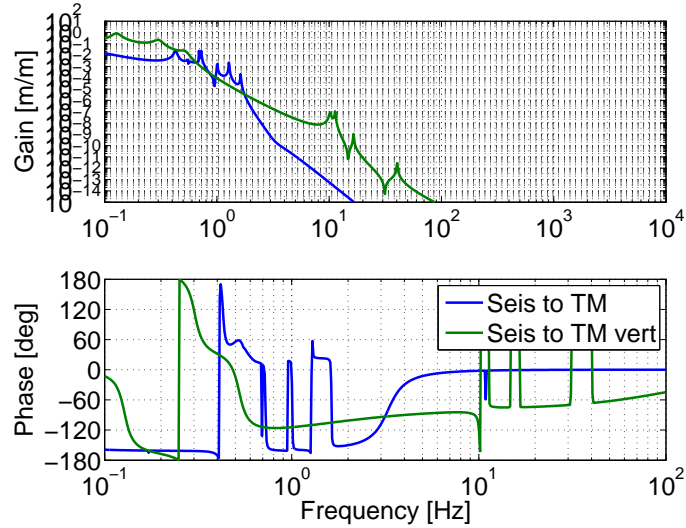


Figure 3: BS seismic noise suppression ratio.

2.4 Seismic noise

The Kamioka seismic noise used in the modeling is plotted below.

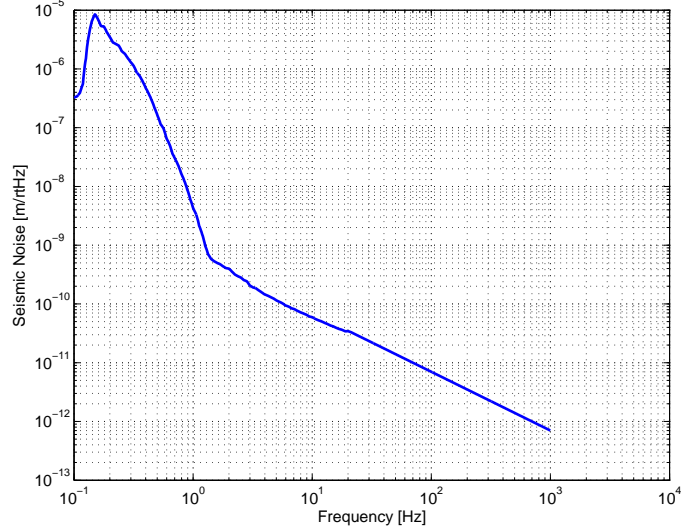


Figure 4: Kamioka seismic noise.

2.5 Coil drivers

We have two types of coil drivers, the high power one and the low power one. They are basically the copies of [LIGO-D0902747](#) and [LIGO-D070481](#), respectively, but has different dewhitening filters compared with LIGO ones. The high power one and the low power one both have switchable three-stage dewhitening filters with pole @ 1 Hz and zero @ 10 Hz (gain of 1 at DC). In the simulation, all the dewhitening filters are turned on. The high power one is used for IM coils and the low power one is used for TM coils.

V-I conversion factor for each coil driver when all the dewhitening filters are turned off is plotted in Fig. 5. The resistance of the coil is not included here, but it is included in the model (as $13\ \Omega$). The resistances are $80\ \Omega$ for the high power one, and $7.8 \times 10^3\ \Omega$ for the low power one.

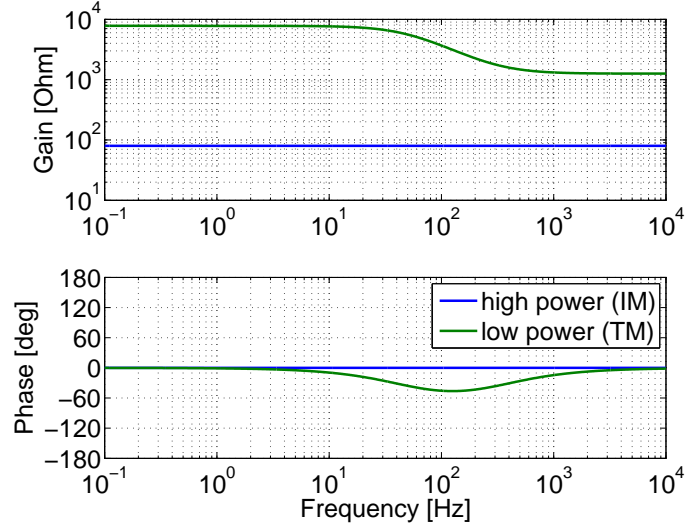


Figure 5: Inverse of V-I conversion factors for high power and low power coil drivers.

Noises of coil drivers used in the model are plotted below, as input equivalent noise to the V-I conversion stage. The numbers come from [LIGO-T080014](#) and [LIGO-T0900233](#).

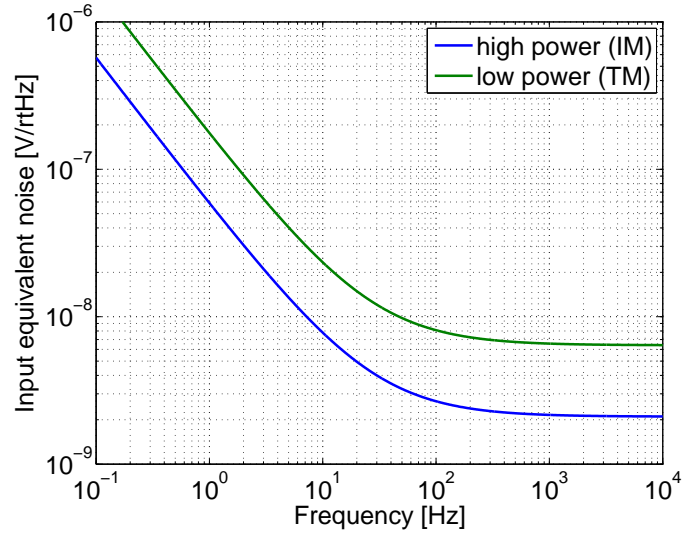


Figure 6: Input equivalent coil driver noise spectra.

2.6 DAC

DAC used for KAGRA is 16 bit and has the range of ± 20 V. The DAC noise is plotted below.

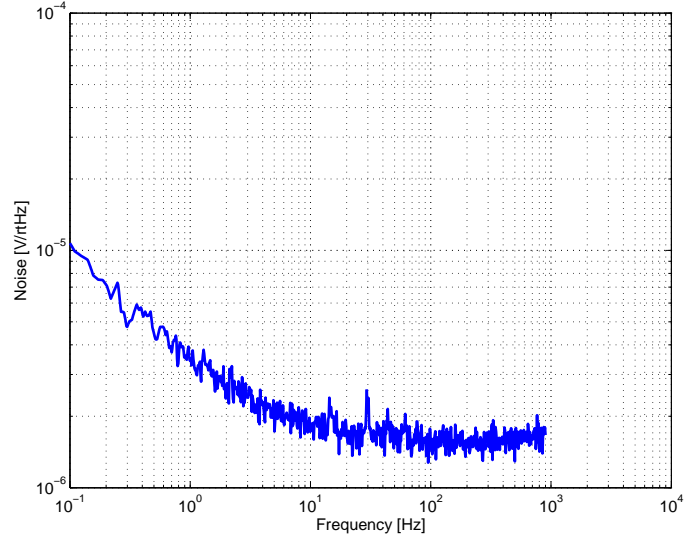


Figure 7: DAC noise.

3 Results for BS

Resulting plots for BS actuator noise modeling are shown. BS is suspended by a Type-B suspension, but differs from other Type-B's since the mirror mass is heavier.

3.1 Openloop transfer function

The openloop transfer function is shown below.

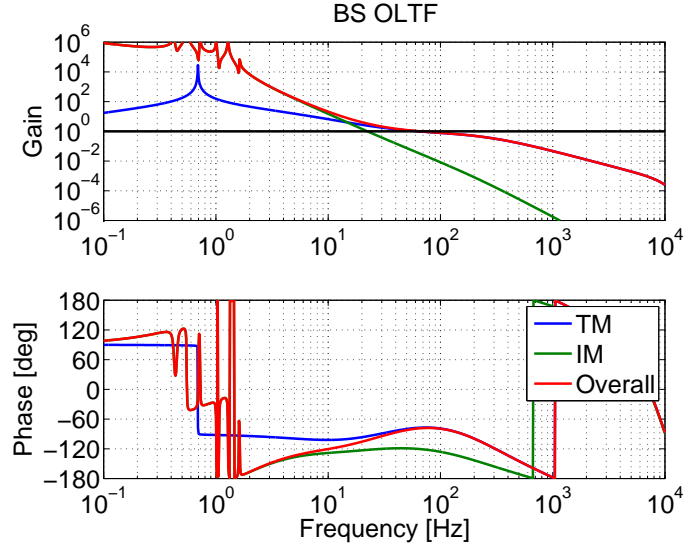


Figure 8: Openloop transfer functions for the BS length servo.

3.2 Noise budget

The displacement noise budget and the actuator noise budget are shown below. The lines labeled "Requirement" show the BS displacement noise requirement in Ref. [7], and the safety factor of 10 is included.

As you can see, the seismic noise and the actuator noise barely meet the requirement above 10 Hz. The most contributing noise among the actuator noises is the noise from TM coil driver.

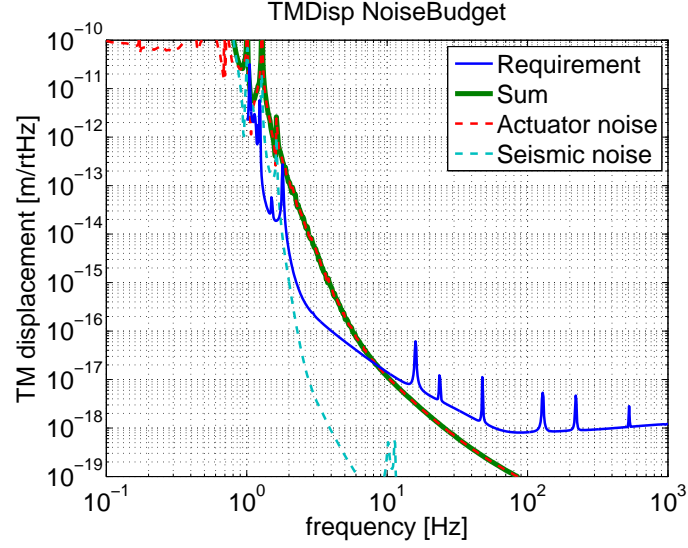


Figure 9: Displacement noise budget for BS.

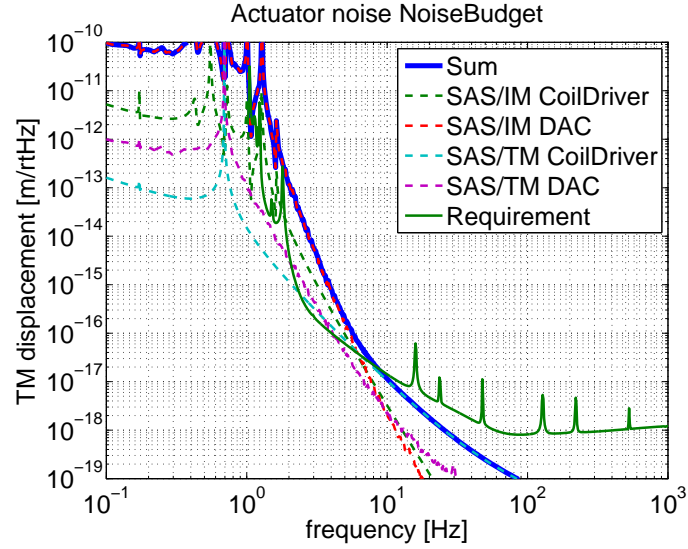


Figure 10: Actuator noise budget for BS.

3.3 Feedback signal saturation check

The spectra of feedback signals for IM and TM are shown in the figures below. The blue lines labeled "DAC limit" shows the DAC range (2^{16}).

As you can see, RMS of the feed back signals do not exceed the DAC limit. So, we can reduce the actuation efficiency for BS to be more safe in actuator noise.

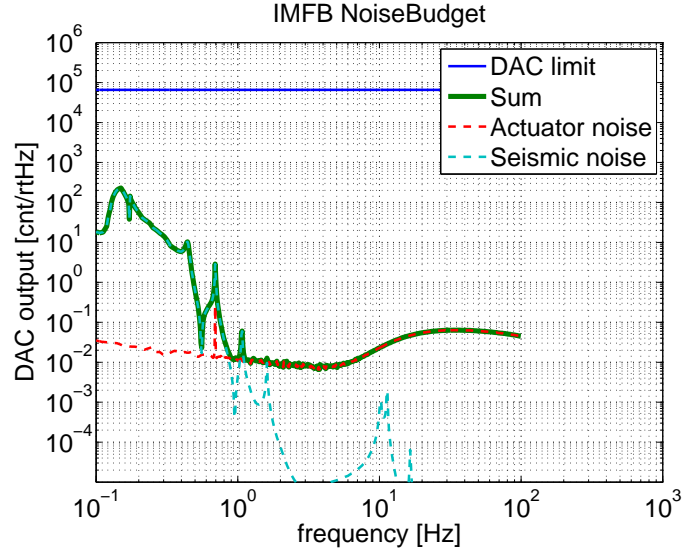


Figure 11: Spectra of feedback signals for the BSIM.

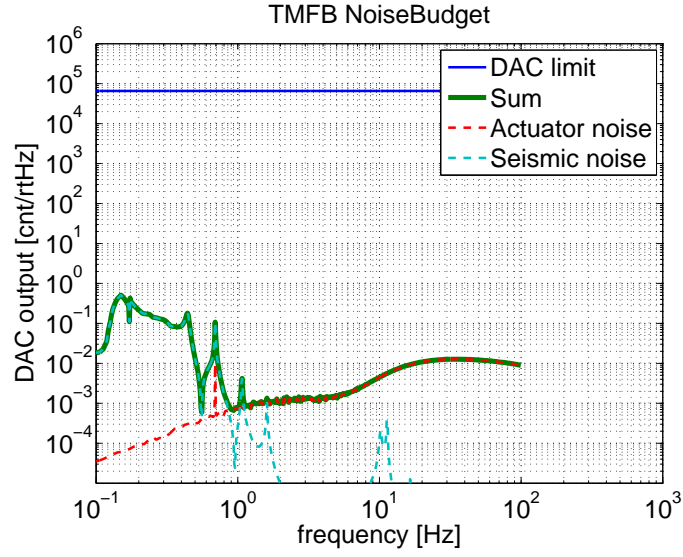


Figure 12: Spectra of feedback signals for the BSTM.

4 Results for SRM

Resulting plots for SRM actuator noise modeling are shown. SRM is suspended by a Type-B suspension. Although displacement noise requirements for SRM and BS is similar, SRM is more severe to the actuator noise since SRM is lighter than BS.

4.1 Noise budget

The displacement noise budget and the actuator noise budget are shown below.

As you can see, the seismic noise meet the requirement above 10 Hz, but the **actuator noise does not**. The most contributing noise among the actuator noises is the noise from TM coil driver. **We should reduce actuation efficiency for SRM TM by more than a factor of 2.**

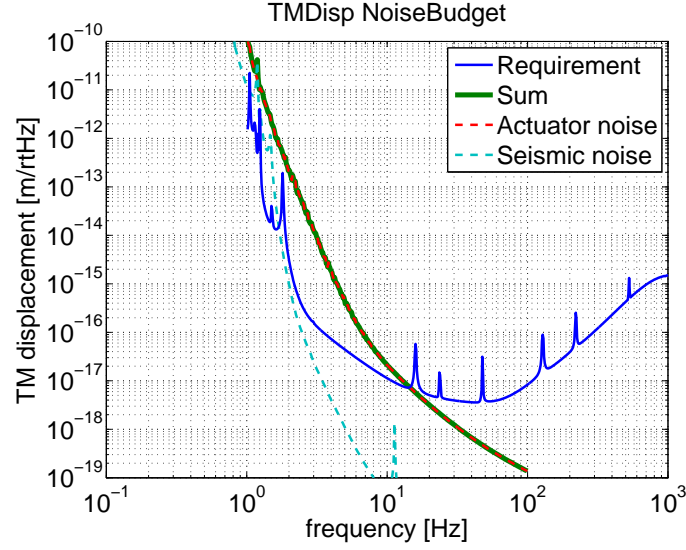


Figure 13: Displacement noise budget for SRM.

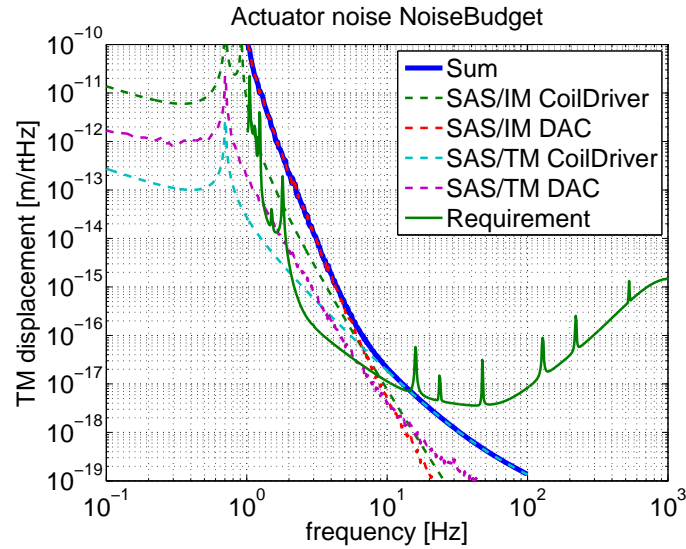


Figure 14: Actuator noise budget for SRM.

4.2 Feedback signal saturation check

The spectra of feedback signals for IM and TM are shown in the figures below.

As you can see, RMS of the feed back signals do not exceed the DAC limit. So, we can reduce the actuation efficiency for SRM to meet the actuator noise requirement.

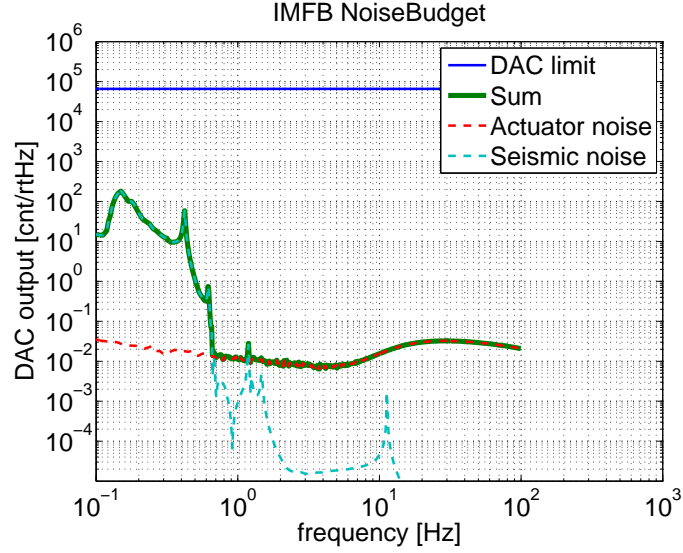


Figure 15: Spectra of feedback signals for the SRMIM.

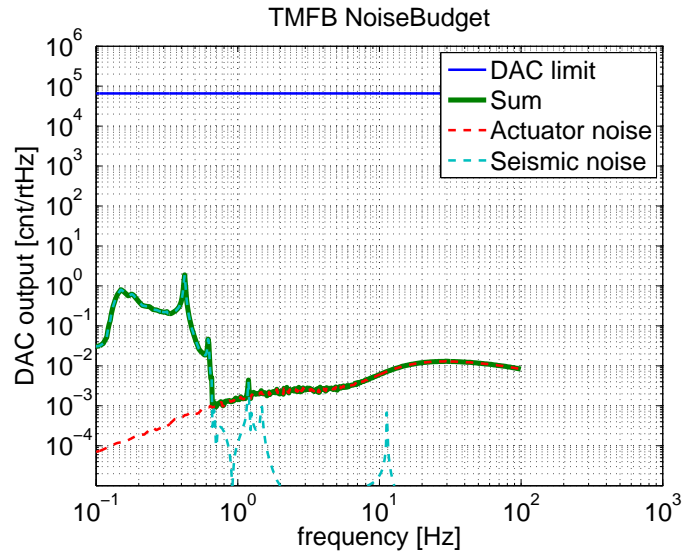


Figure 16: Spectra of feedback signals for the SRMTM.

5 Results for PRM

Resulting plots for PRM actuator noise modeling are shown. PRM is suspended by a Type-Bp suspension. Type-Bp suspension is basically Type-B, but upper stage (Standard Filter) is fixed. So, actuation transfer functions are the same as SRM ones, but seismic suppression ratio is different.

5.1 Noise budget

The displacement noise budget and the actuator noise budget are shown below.

As you can see, the seismic noise and the actuator noise well meet the requirement above 10 Hz.

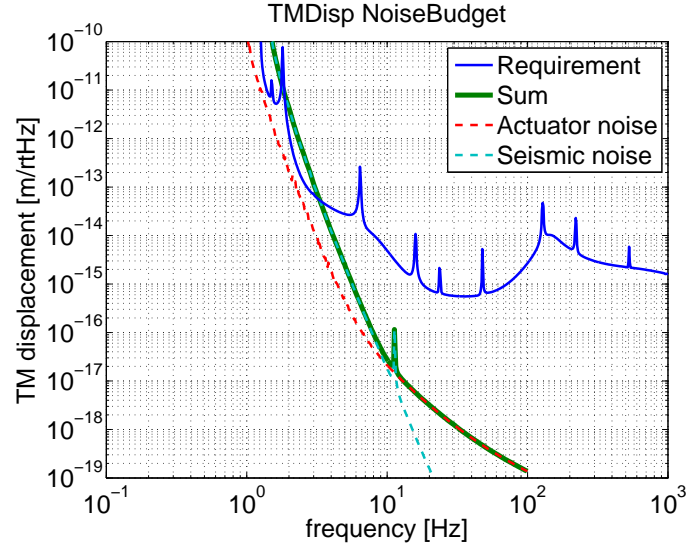


Figure 17: Displacement noise budget for PRM.

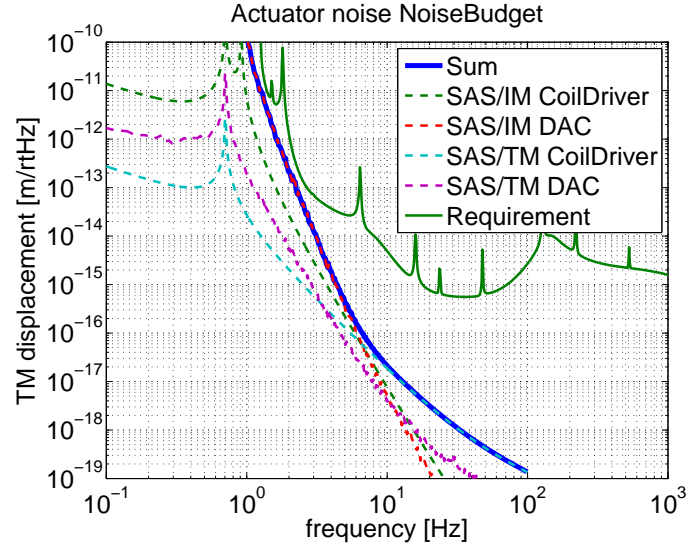


Figure 18: Actuator noise budget for PRM.

5.2 Feedback signal saturation check

The spectra of feedback signals for IM and TM are shown in the figures below.

As you can see, RMS of the feed back signals do not exceed the DAC limit.

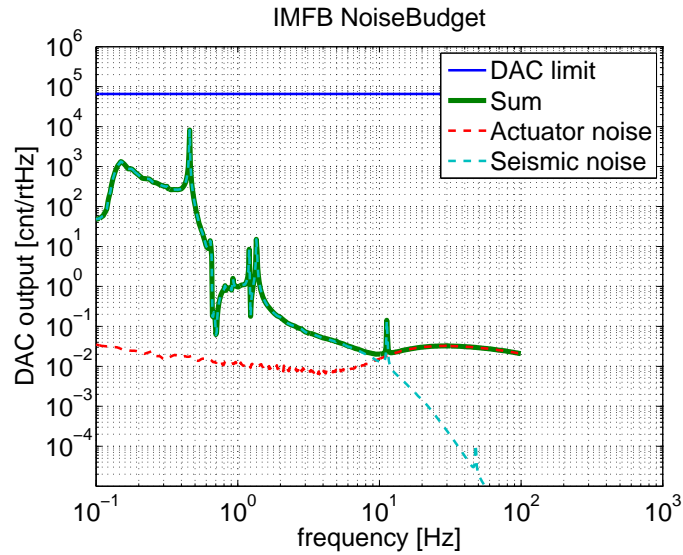


Figure 19: Spectra of feedback signals for the PRMIM.

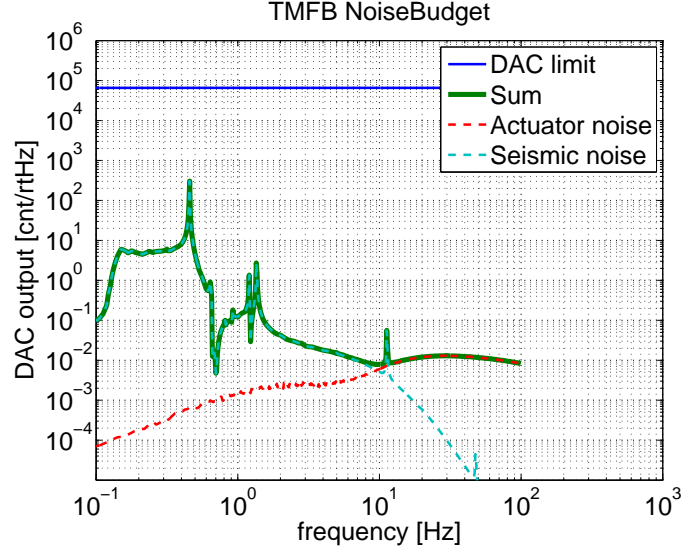


Figure 20: Spectra of feedback signals for the PRMTM.

6 Results for IMC suspensions

Resulting plots for actuator noise modeling for IMC suspensions are shown. IMC mirrors are suspended by Type-C suspension. Type-C suspension is a double pendulum fixed on a three-stage stack. There are no actuators for IM. Whitening and dewhitening filters are not used for coils for IMC suspensions. We will use different coil drivers from Type-B suspensions for IMC suspensions, but here I assumed the same inout noise level (in $V/\sqrt{\text{Hz}}$). Also, vertical noise coupling is not included at this point.

6.1 Noise budget

The displacement noise budget and the actuator noise budget are shown below. The displacement noise requirement for the IMC suspensions comes from the frequency noise requirement after the frequency stabilization servo using IMC length.

As you can see, the seismic noise and the actuator noise well meet the requirement above 10 Hz.

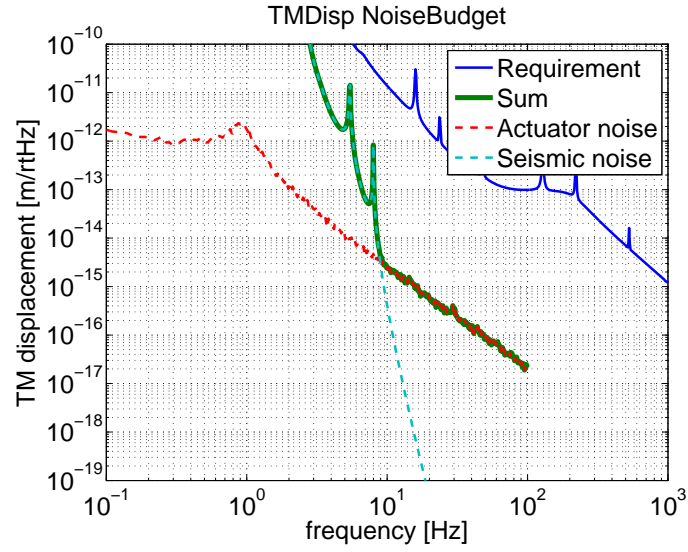


Figure 21: Displacment noise budget for IMC.

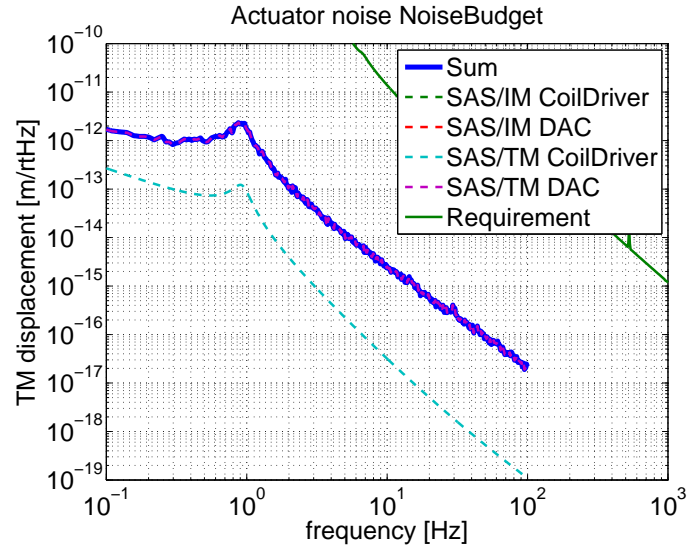


Figure 22: Actuator noise budget for IMC.

6.2 Feedback signal saturation check

The spectra of feedback signals for IM and TM are shown in the figures below.

As you can see, RMS of **the feed back signals saturate the DAC limit**.

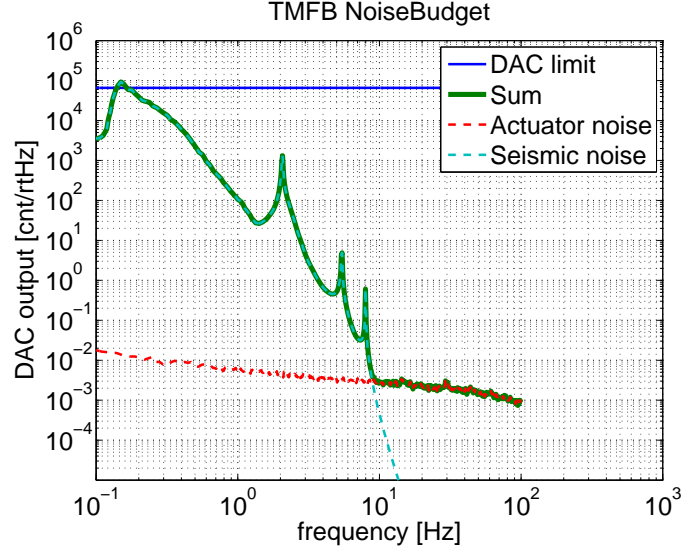


Figure 23: Spectra of feedback signals for the IMCTM.

7 Results for ITM and ETM

To be calculated. Waiting for coil-magnet design.

8 Magnetic noise coupling

We also have to check the magnetic noise coupling for the actuation design study. This calculation for Type-B and Type-Bp suspensions are given in Ref. [8], and we confirmed that the magnetic noise is small enough.

References

- [1] The source code is available from <https://svn.ligo.caltech.edu/svn/aligonoisebudget>. Some instructions are given at <https://awiki.ligo-wa.caltech.edu/aLIGO/NoiseBudget>.
- [2] Yuta Michimura: Summary of Suspension Configurations, JGW-D1503415. <http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/DocDB/ShowDocument?docid=3415>
- [3] Riccardo DeSalvo: Recycler and Beam Splitter suspension structure, JGW-T1100571. <http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/DocDB/ShowDocument?docid=571>
- [4] Takanori Sekiguchi: Type-A SAS Mechanical Model Parameters, JGW-T1302090.

<http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/DocDB/ShowDocument?docid=2090>

- [5] Mark Barton: OSEM Coil/Magnet/Flag Calculation, JGW-T1503239, Table 1.
<http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/DocDB/ShowDocument?docid=3239>
- [6] Takahiro Saito: Mode-cleaner suspension installation, JGW-G1503303, p.18.
<http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/private/DocDB/ShowDocument?docid=3303>
- [7] Yoichi Aso, Yuta Michimura, Kentaro Somiya: KAGRA Main Interferometer Design Document, JGW-T1200913, Figure 4.1 and 4.2.
<http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/DocDB/ShowDocument?docid=913>
- [8] Kenji Ono: Evaluation of BS and RM noise arisen from the AC component of geomagnetism field, JGW-T1503469
<http://gwdoc.icrr.u-tokyo.ac.jp/cgi-bin/DocDB/ShowDocument?docid=3469>