

Status of the input optics for the O3

Masayuki Nakano
Toyama Univ.




Objectives of the input optics

Objectives of the input optics

Provide the stable laser to the main interferometer.


- ✓ The frequency stabilization
- ✓ The intensity stabilization
- ✓ The reduction of the beam jitter
- ✓ The cleaning of the spacial mode of the laser

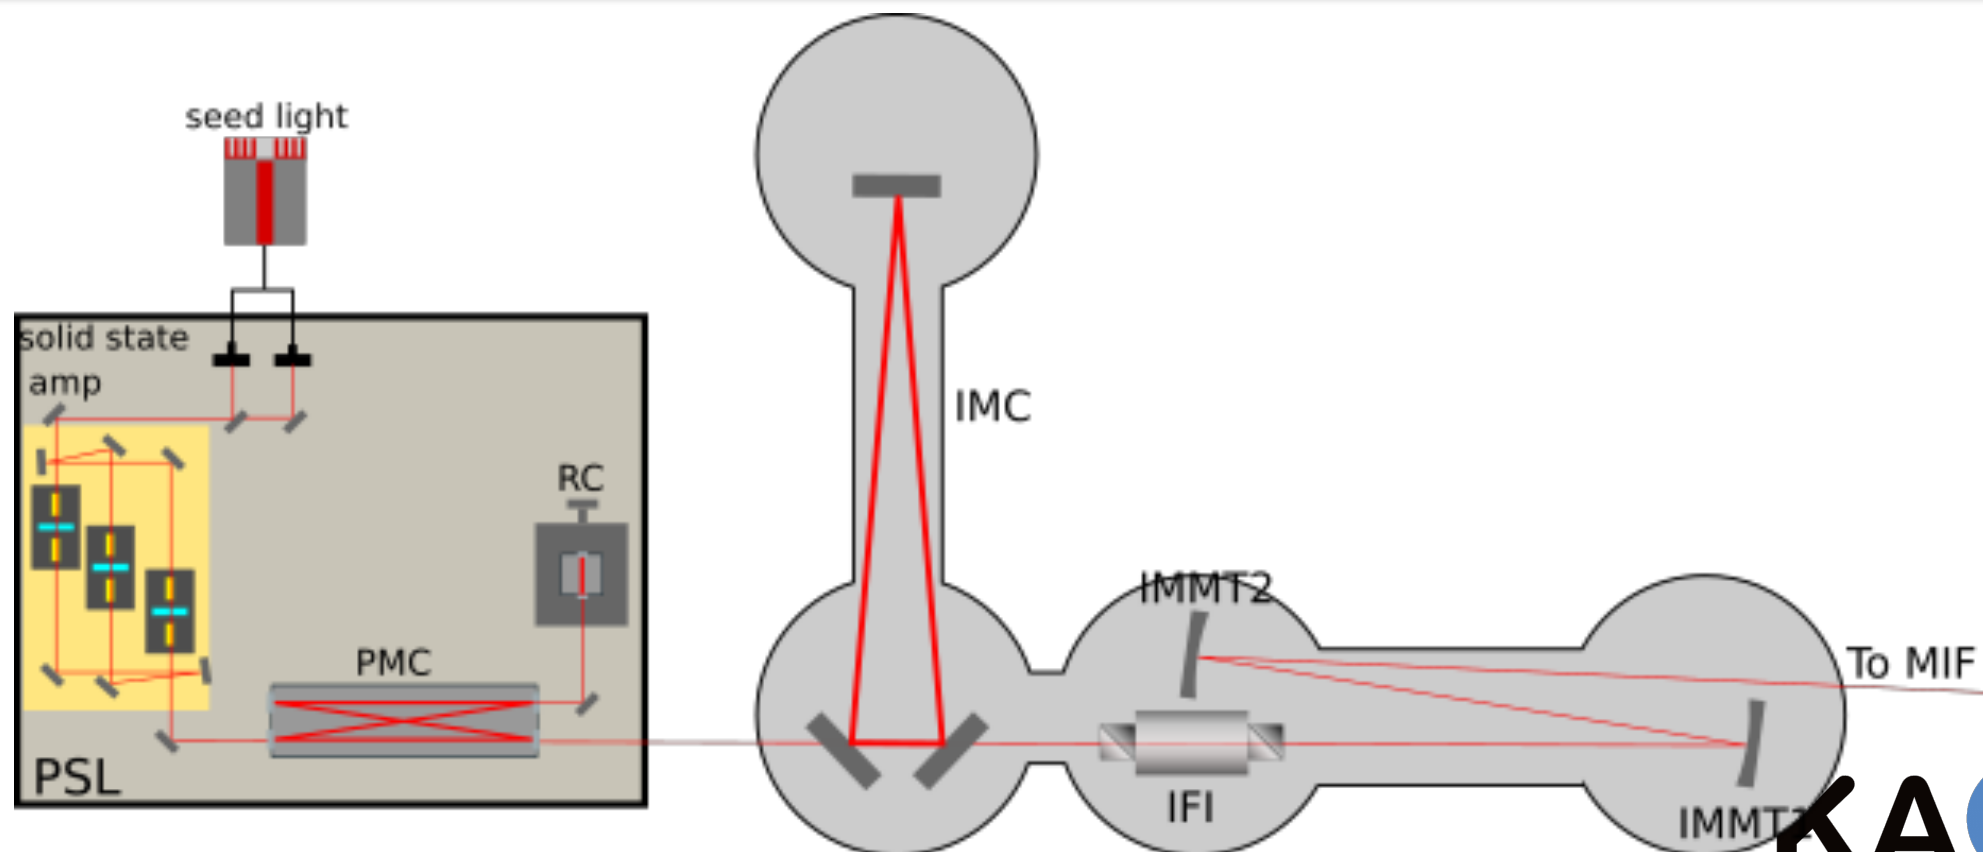

Status of the input optics

- Almost all system has installed.
- The maximum power from the IMC is 4 W so far, with the fiber amplifier output of 10 W
- The alignment control for the input mode cleanser is not finalized yet.
- Although the modulation system using the Mach-Zehnder interferometer has been installed, the displacement noise does not meet the requirement for the O3.
 - ✓ We decided not to use the MZM.

Overview of the input optics

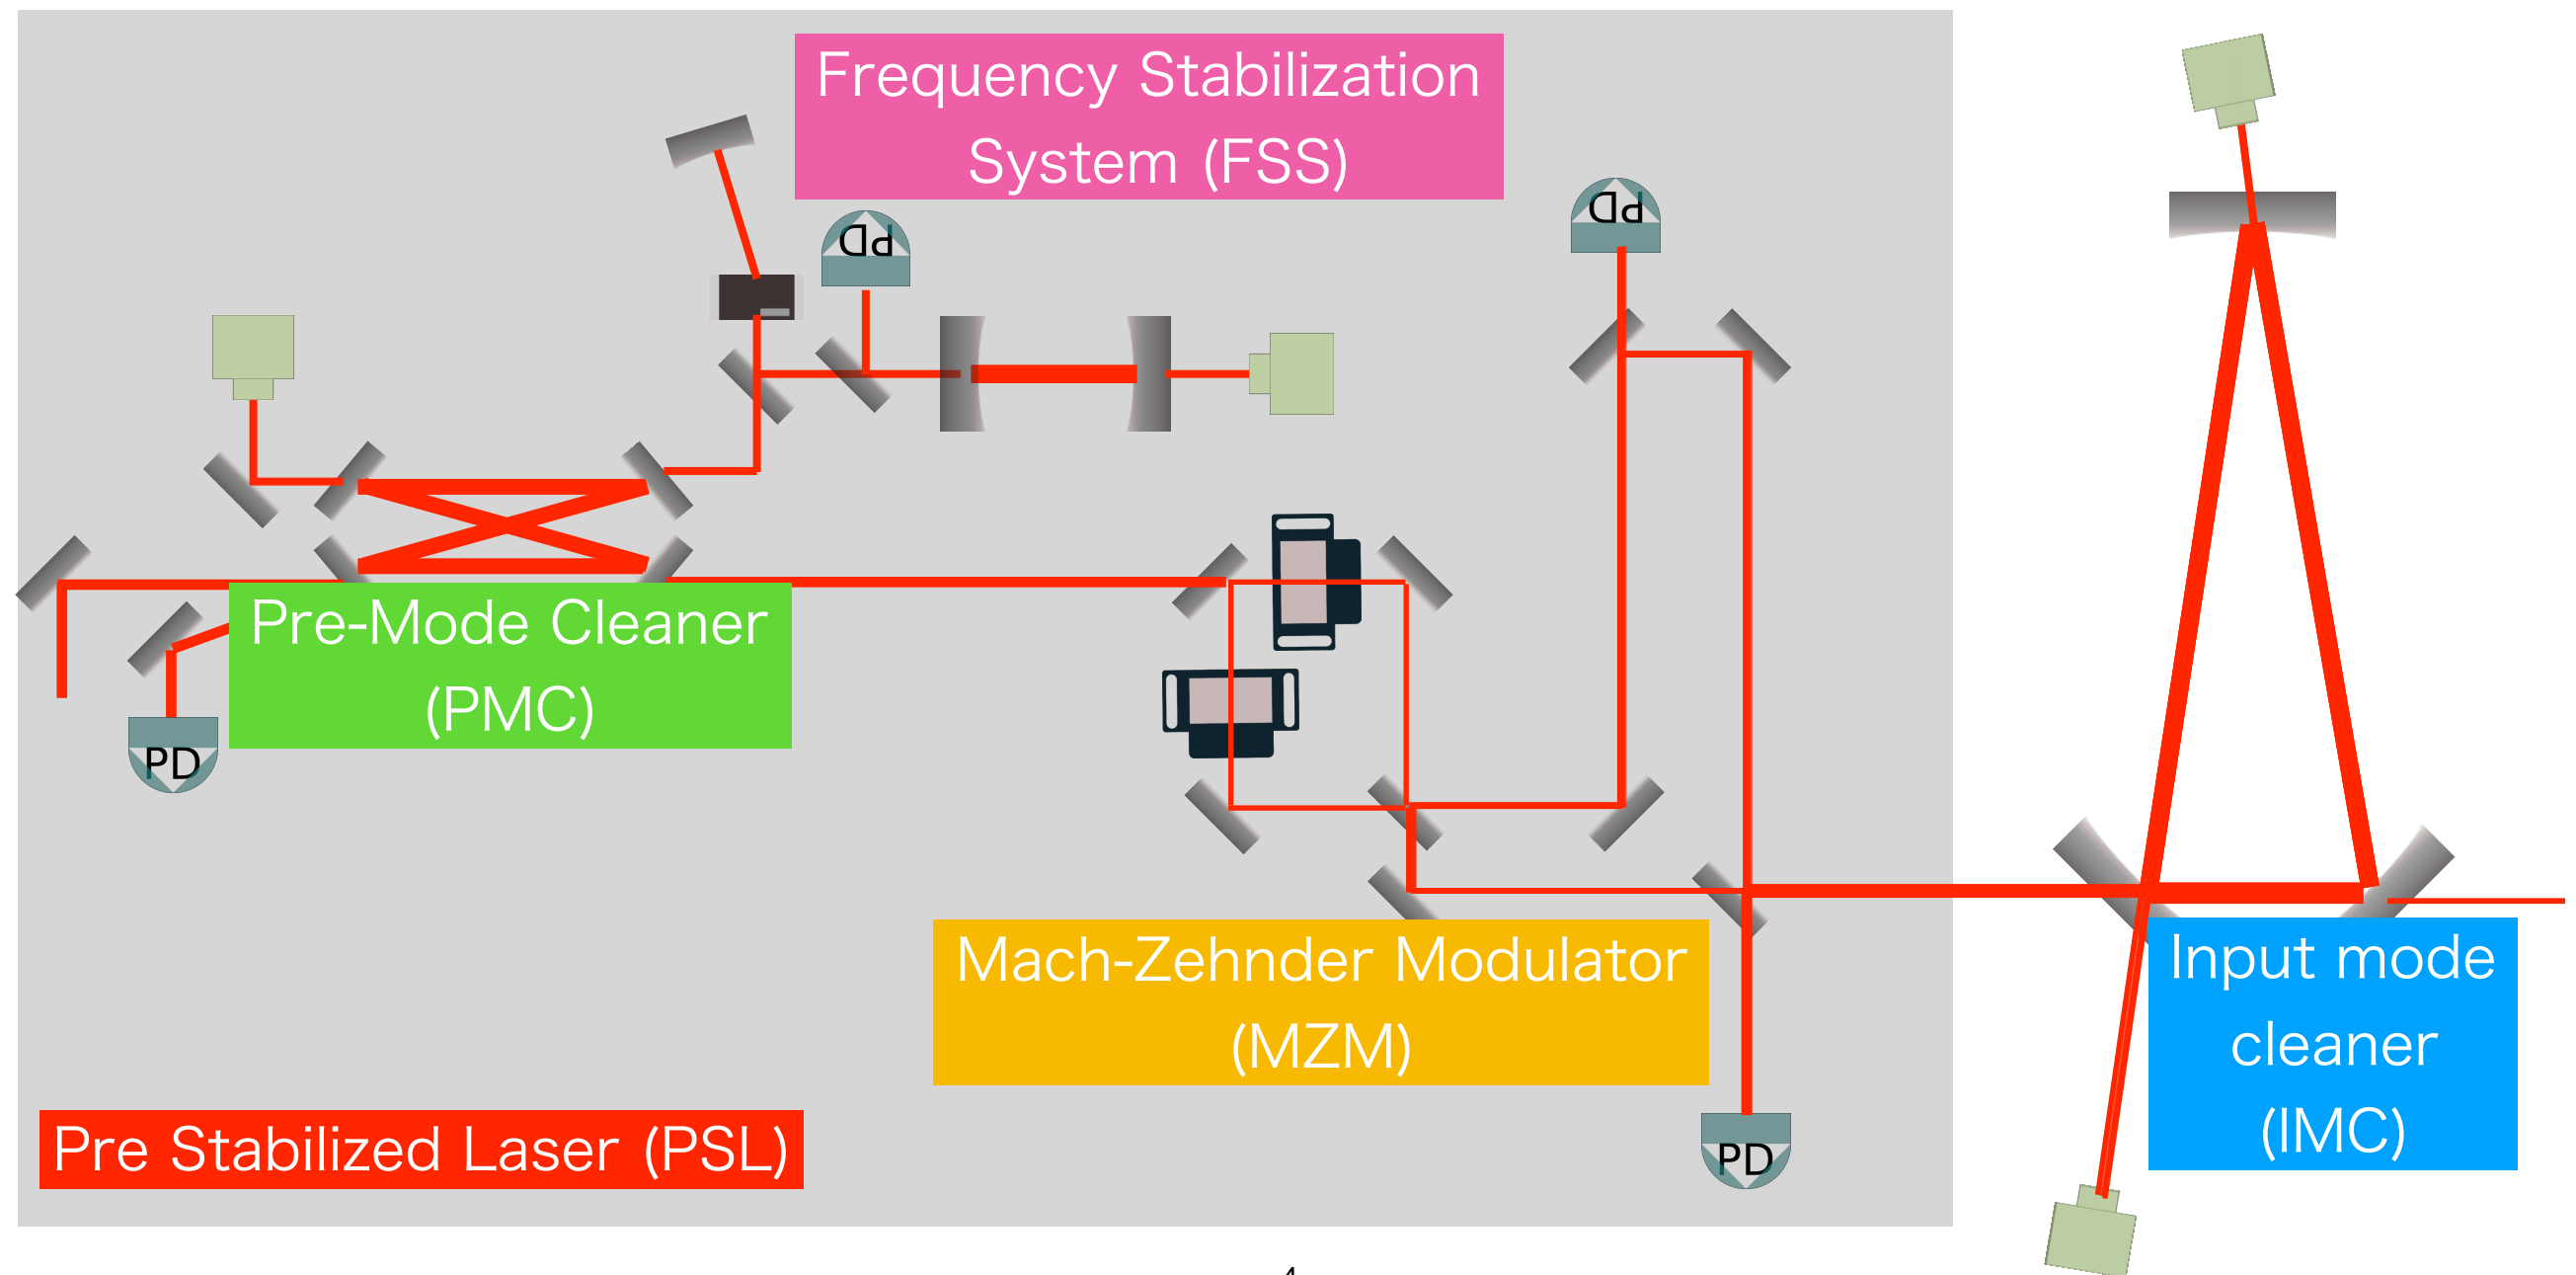

Pre-Stabilized Laser (PSL)




MZM

FSS

PMC


Pre-Mode Cleaner (PMC)

Pre-Mode Cleaner

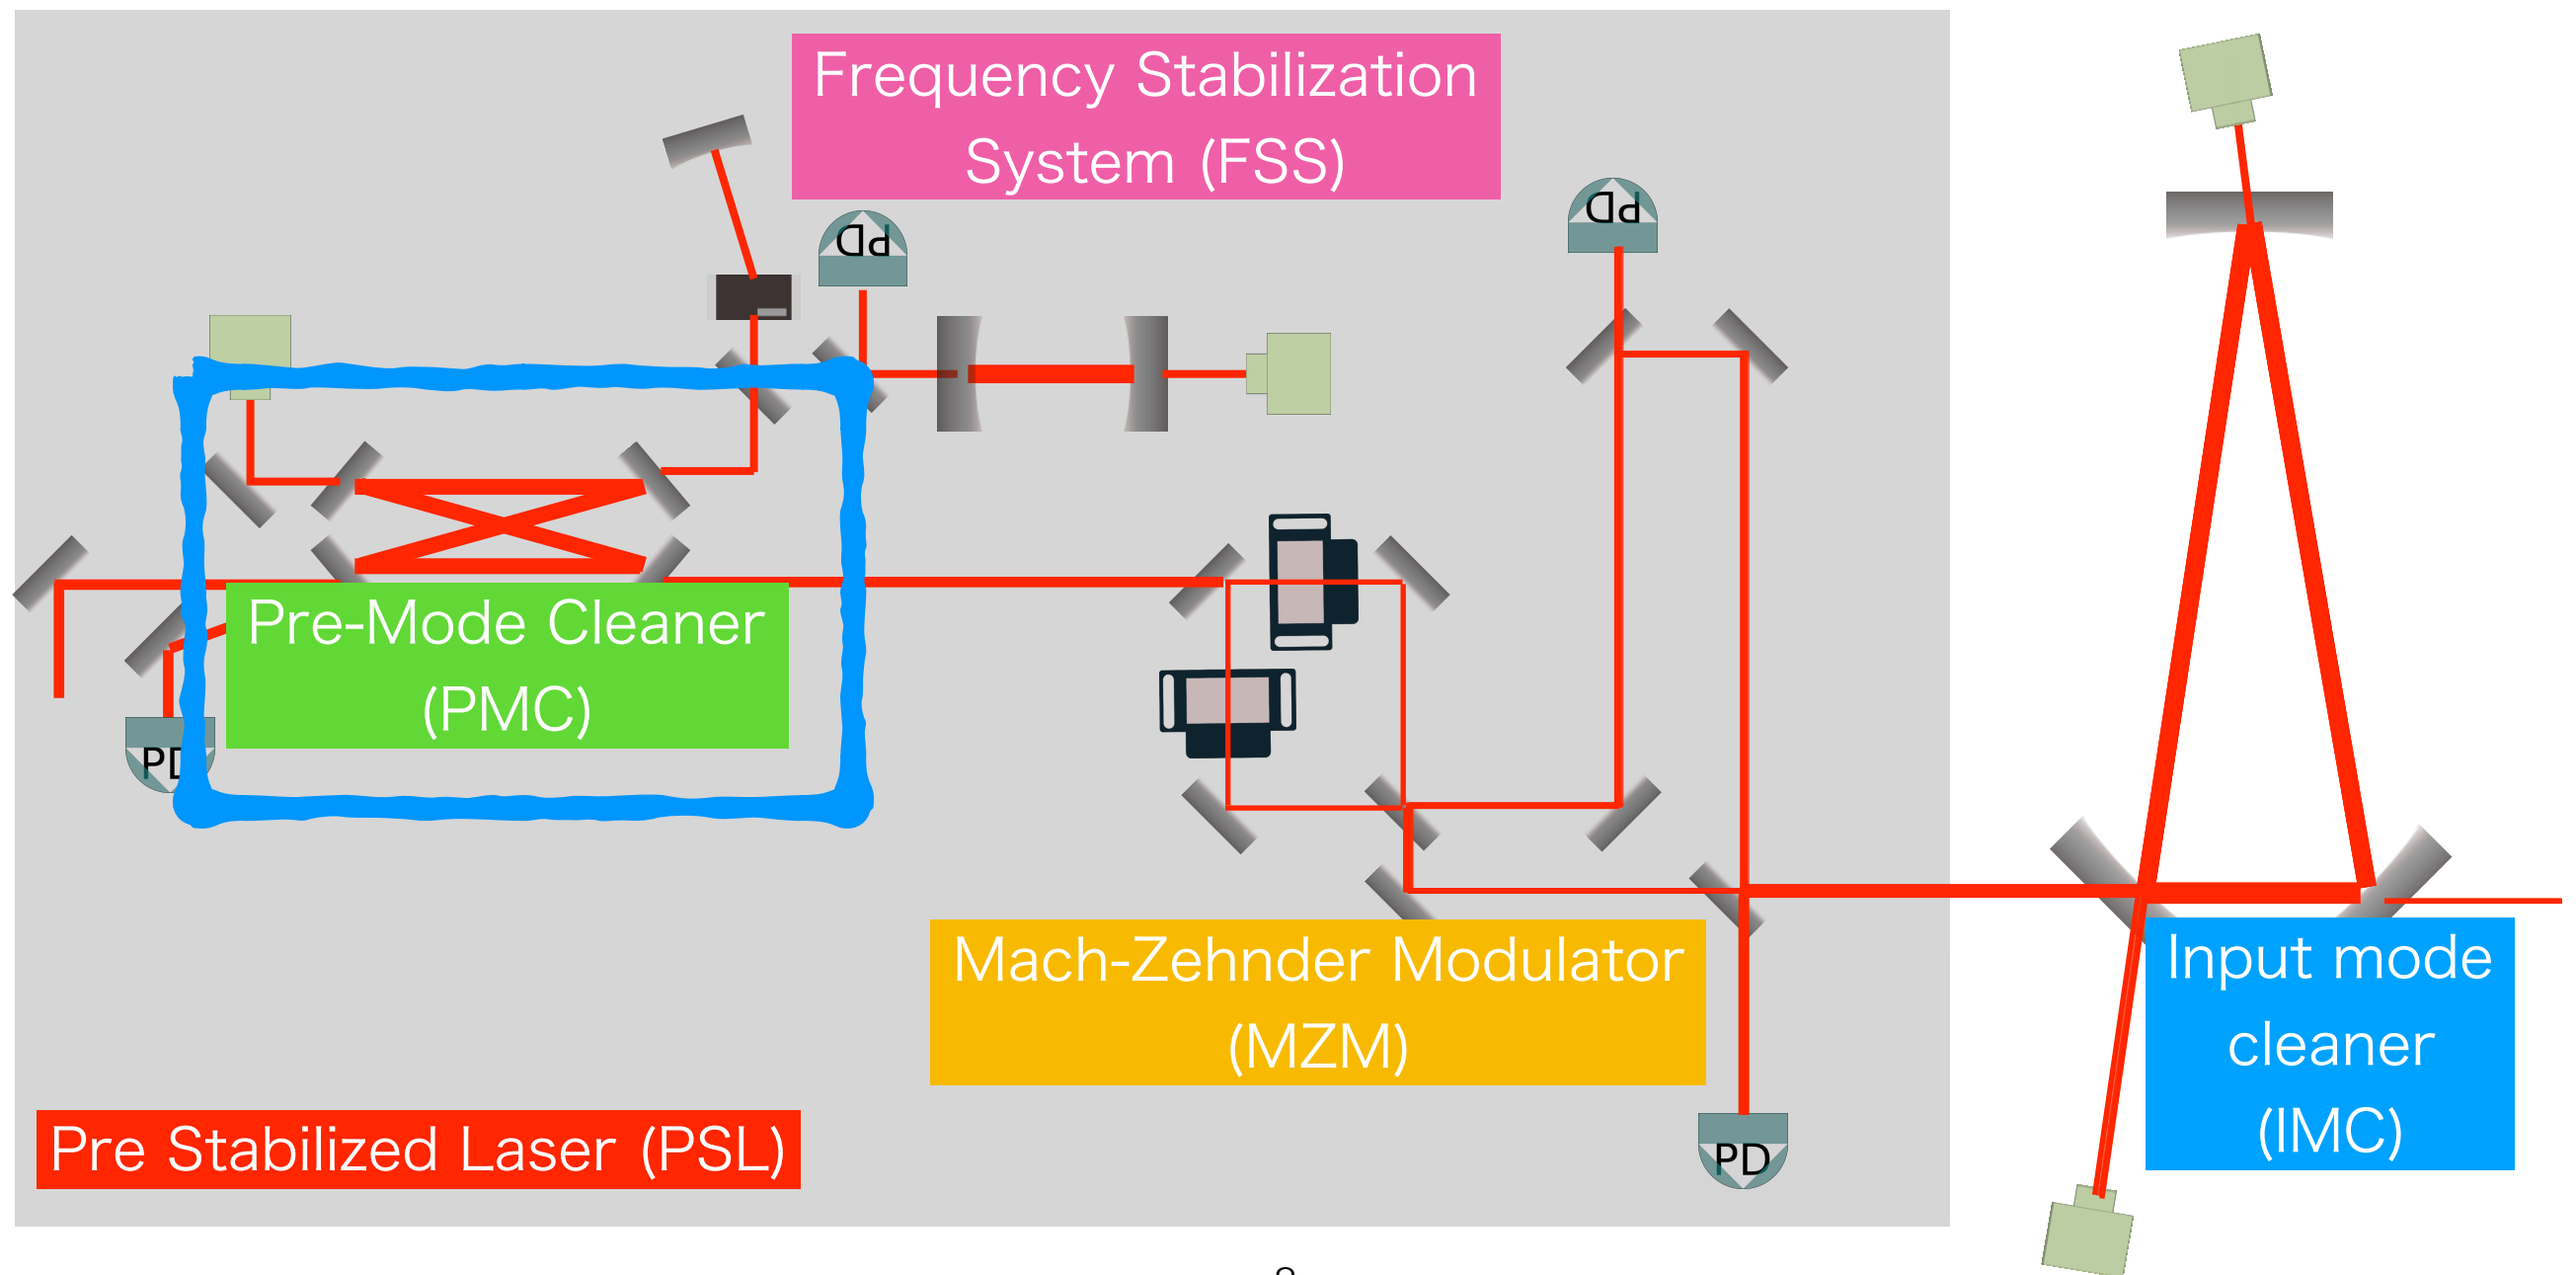


Pre-Mode Cleaner (PMC)

- 2-m long bow-tie shaped cavity.
- Objectives:
 - ✓ Spatial mode cleaning
 - ✓ Beam jitter reduction
 - ✓ RF RAM noise suppression
- Control the Cavity length to follow the laser frequency.

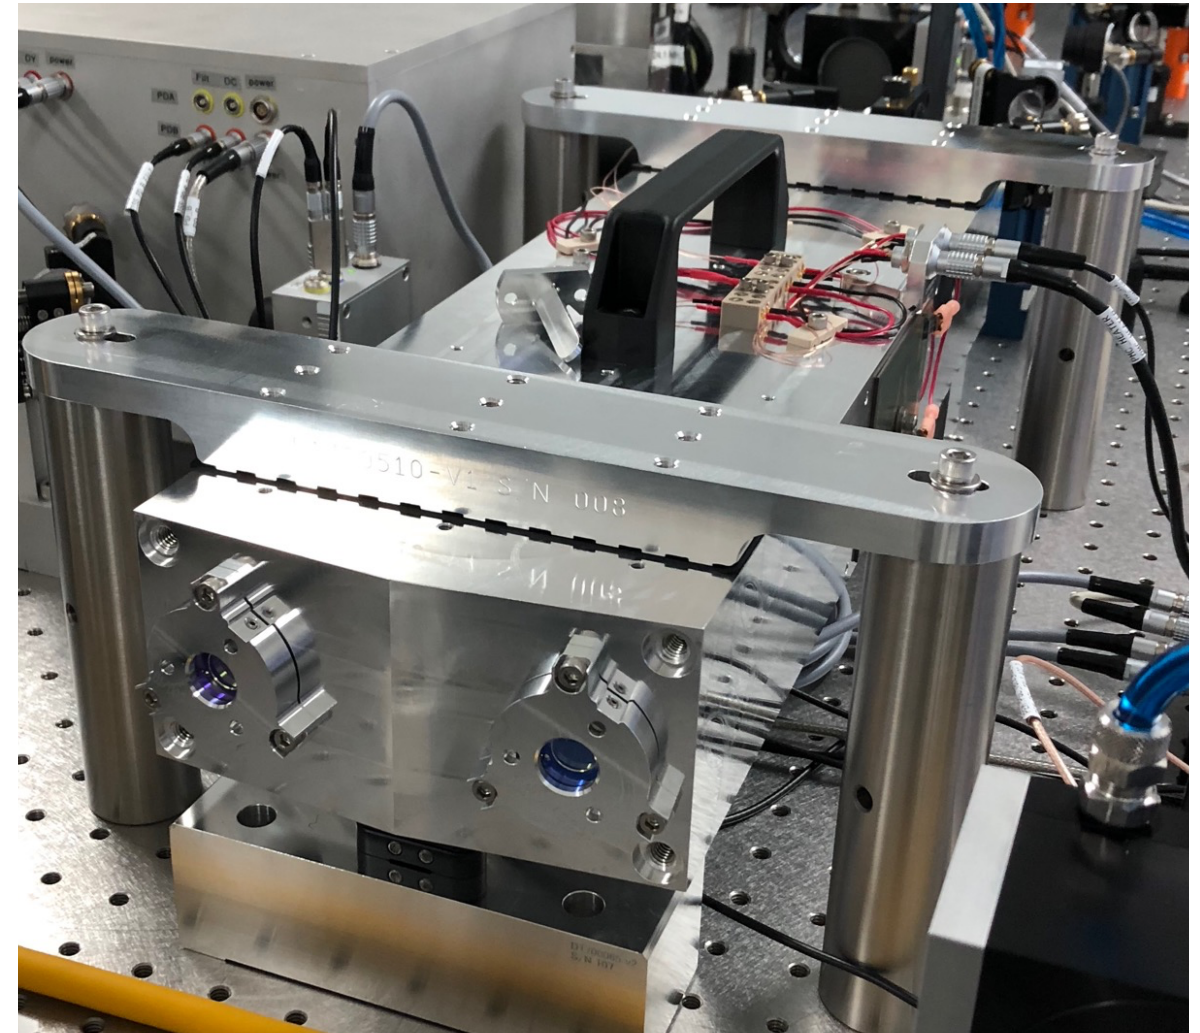


Input Mode Cleaner (IMC) And Frequency Stabilization System(FSS)

IMC and FSS


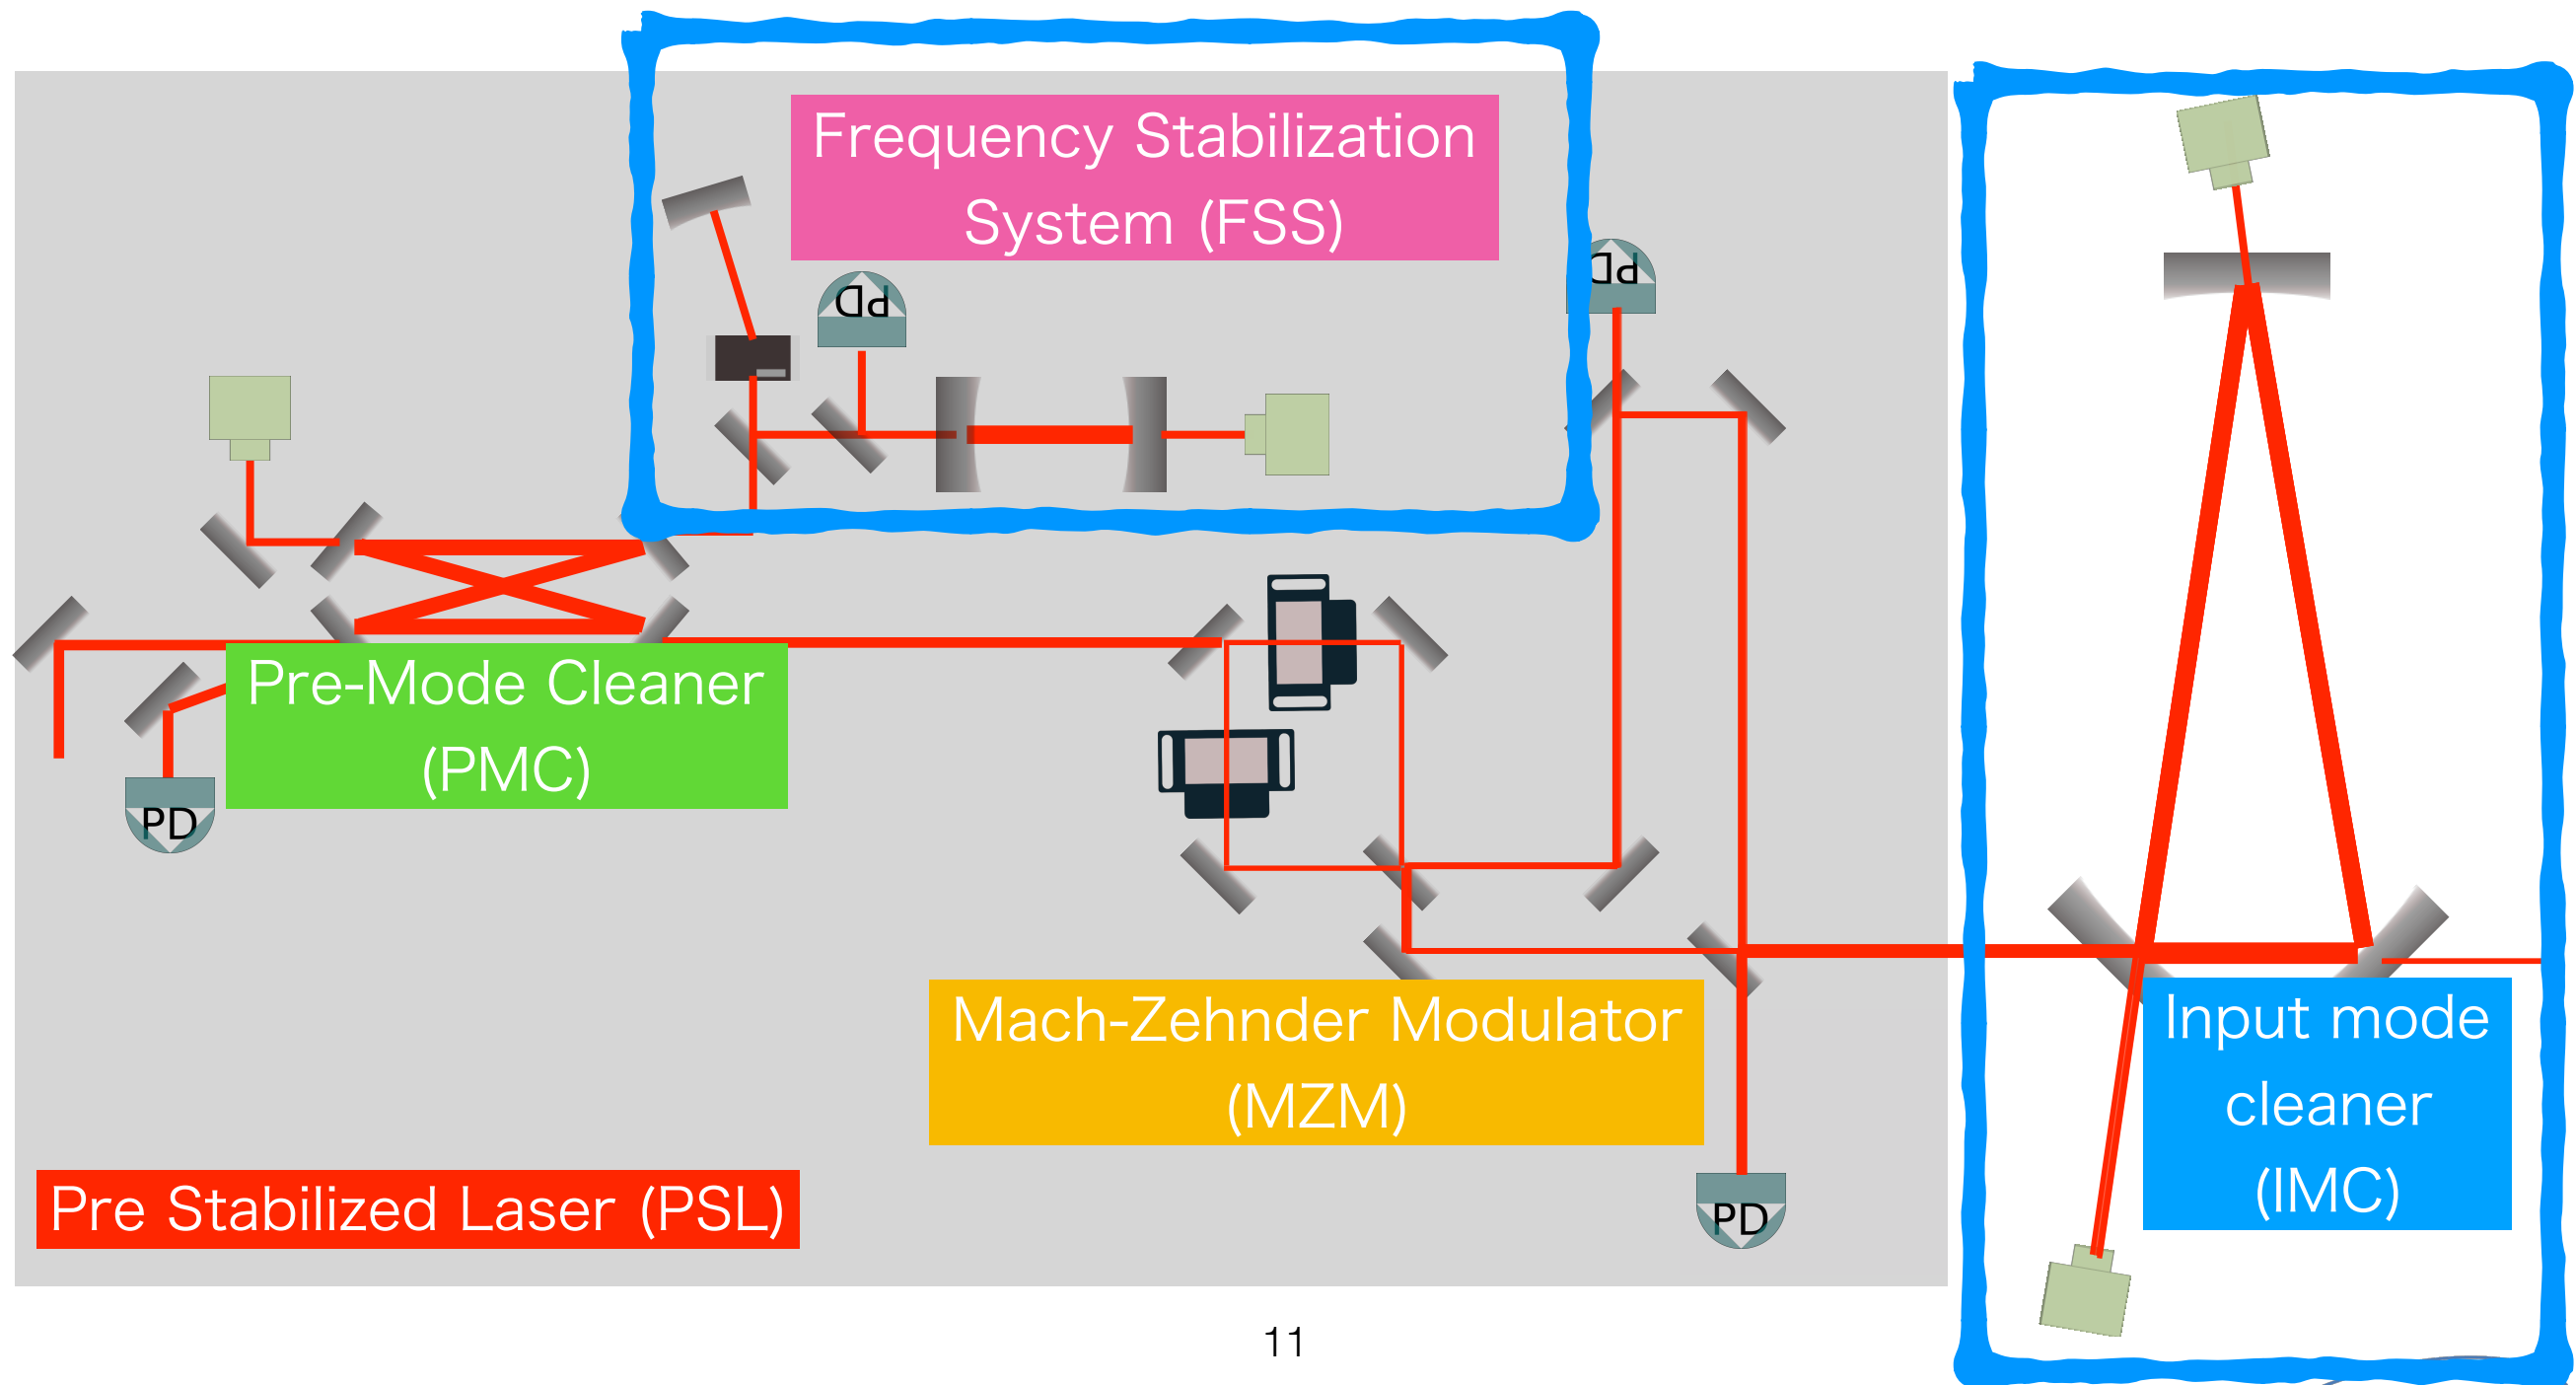


Frequency Stabilization

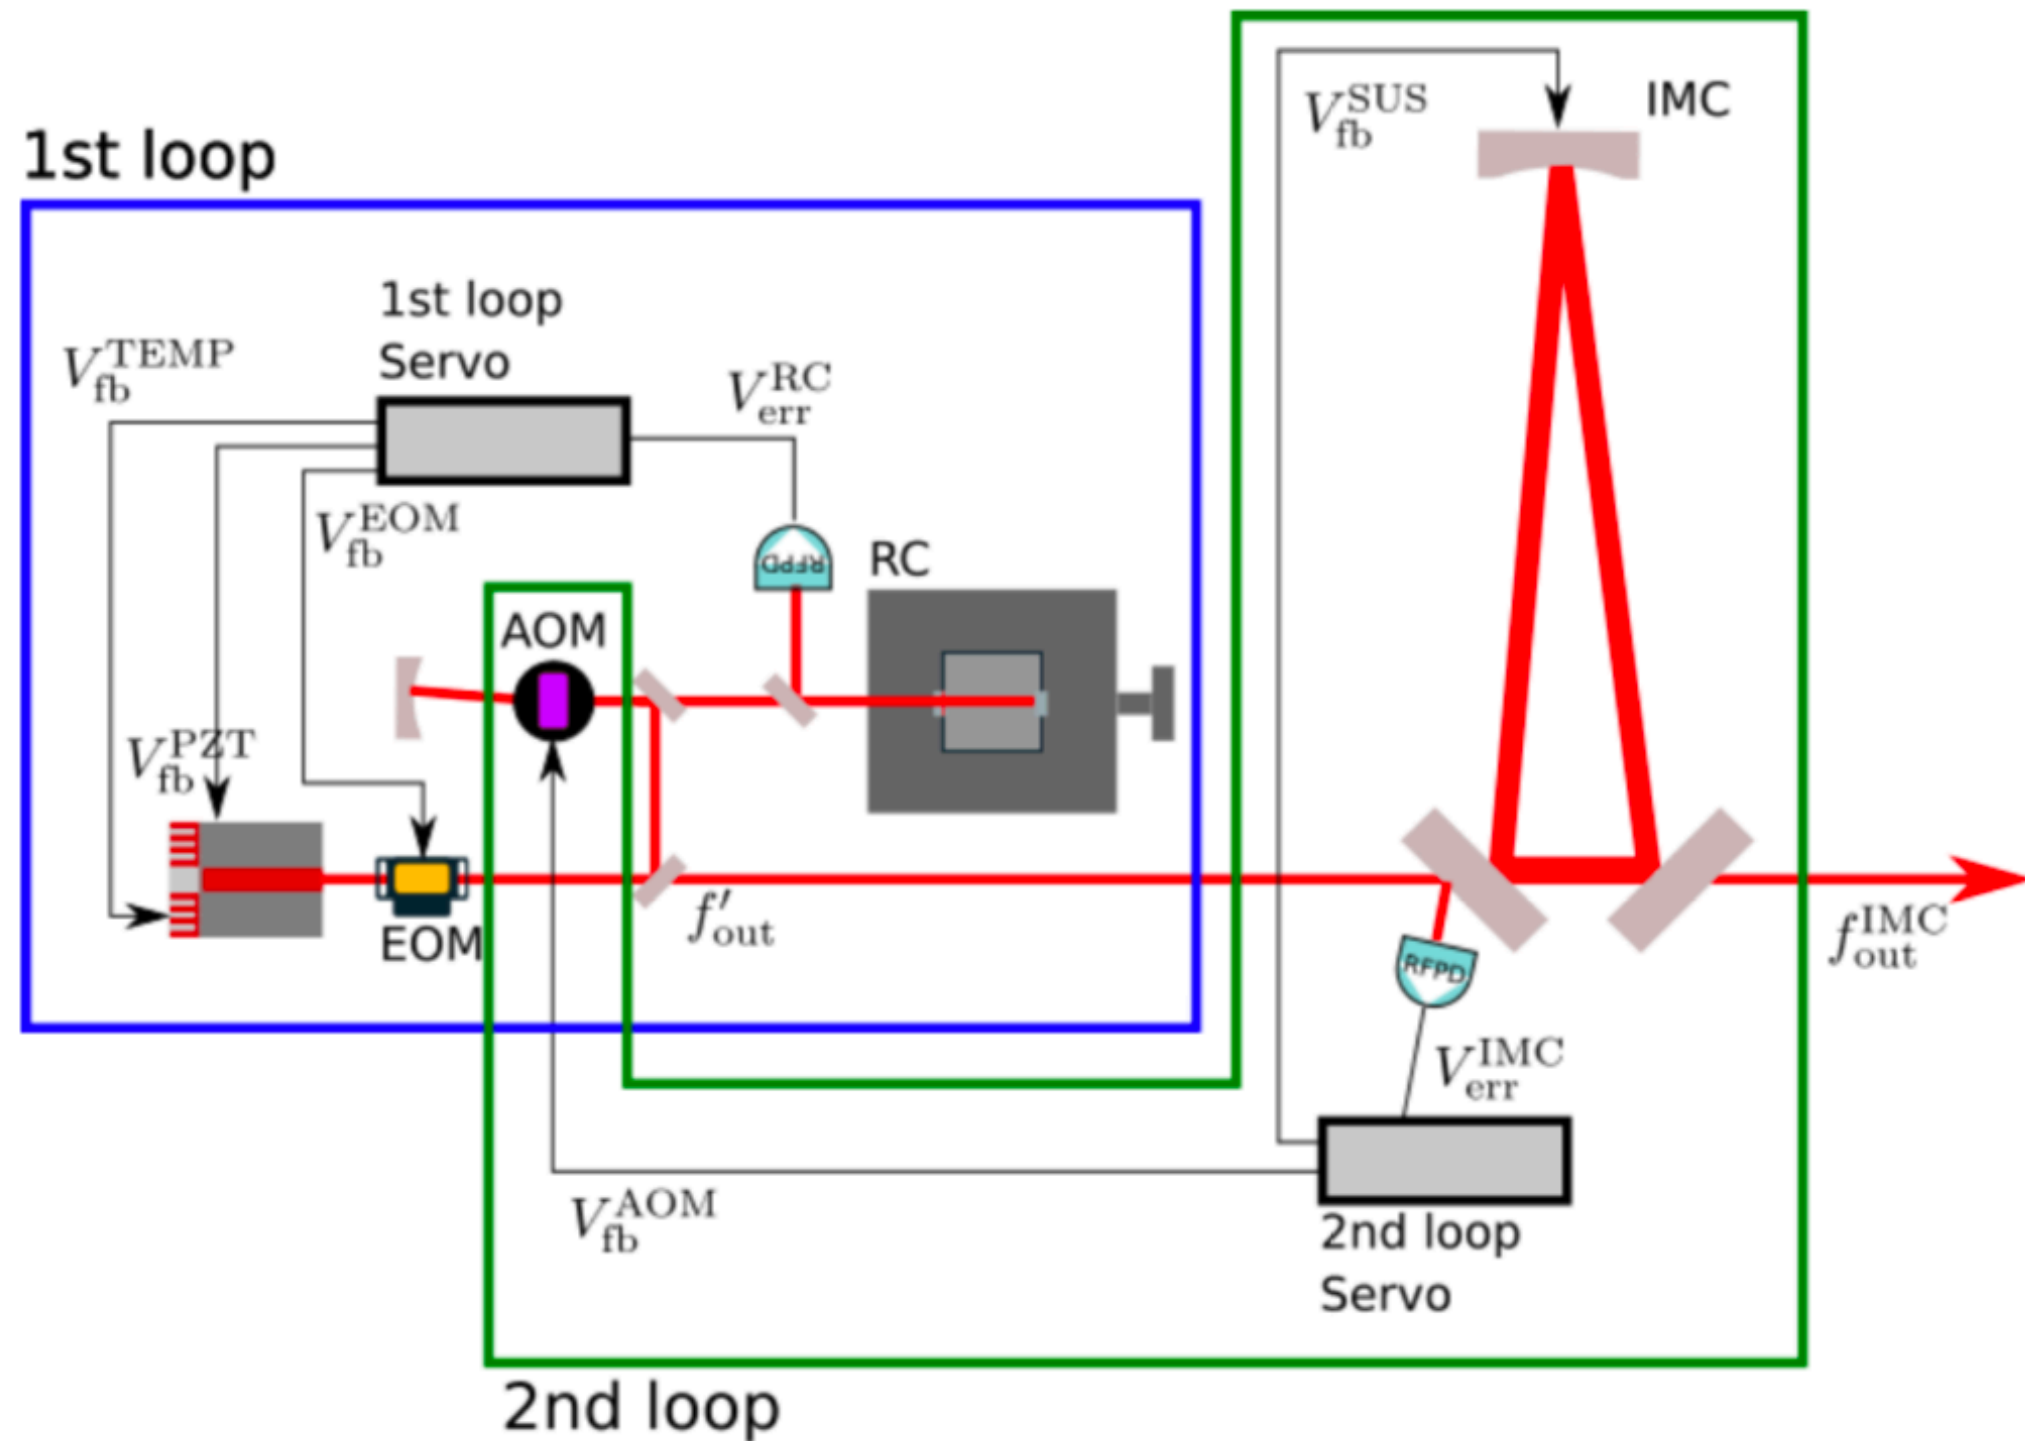




Reference Cavity

- Use the ULE glass linear cavity as the frequency reference for the 1st loop.
 - ✓ The resonance frequency of the cavity is more stable than the laser frequency.
- Control the laser frequency to follow the resonance frequency of the reference cavity.
 - ✓ Slow actuator: Laser temperature
 - ✓ Mid actuator: Laser PZT
 - ✓ Fast actuator: Broadband EOM

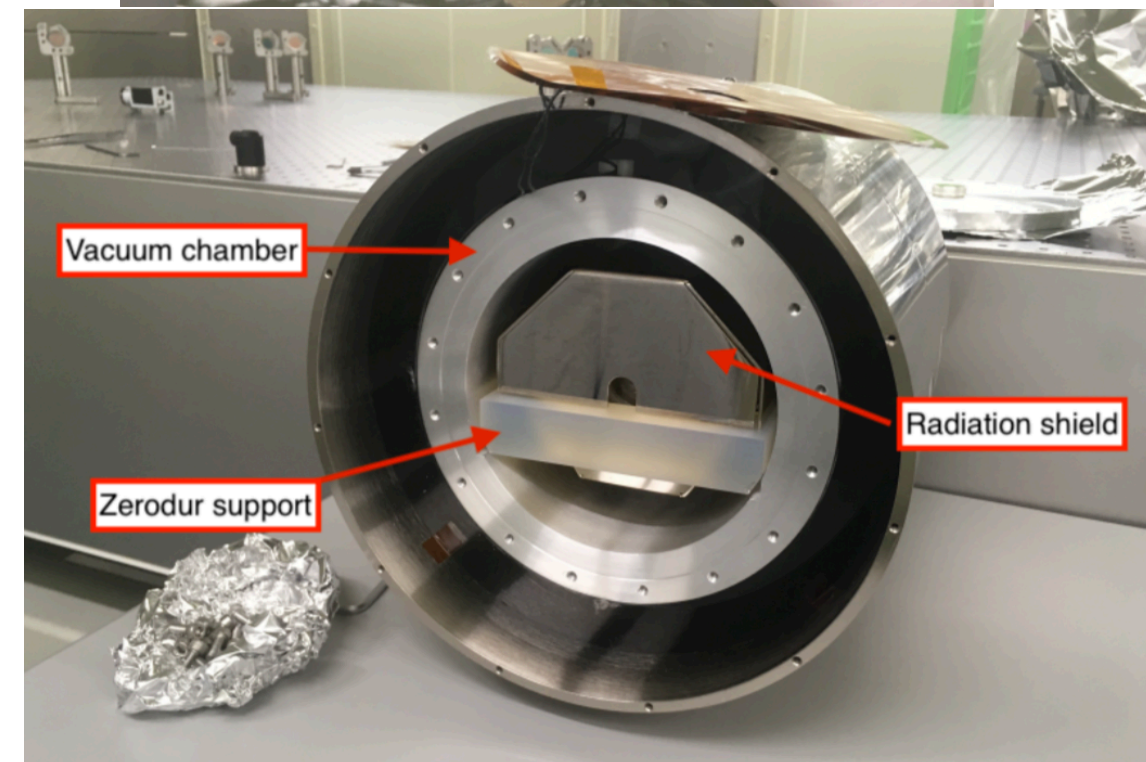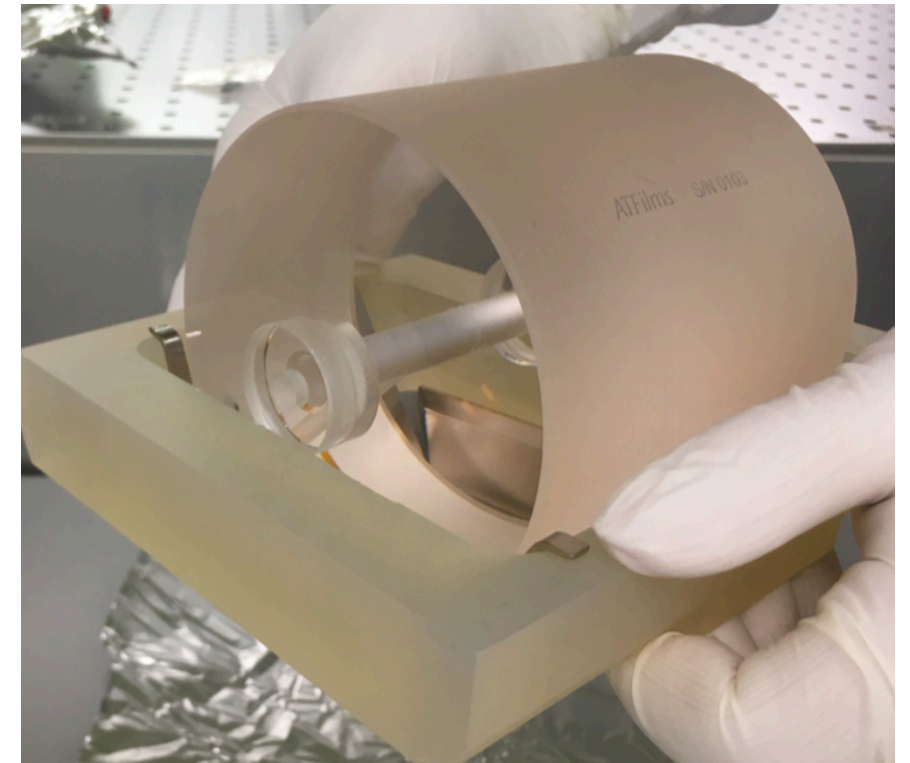


Input Mode Cleaner (IMC)

- Suspended triangular cavity
 - ✓ Cavity length: 25 m
- Objectives
 - ✓ The spacial mode cleaning.
 - ✓ The frequency reference for the FSS.
 - ✓ The beam jitter reduction
- The laser frequency is controlled to follow the resonance frequency of the IMC.
- At low frequencies, the cavity length is controlled.

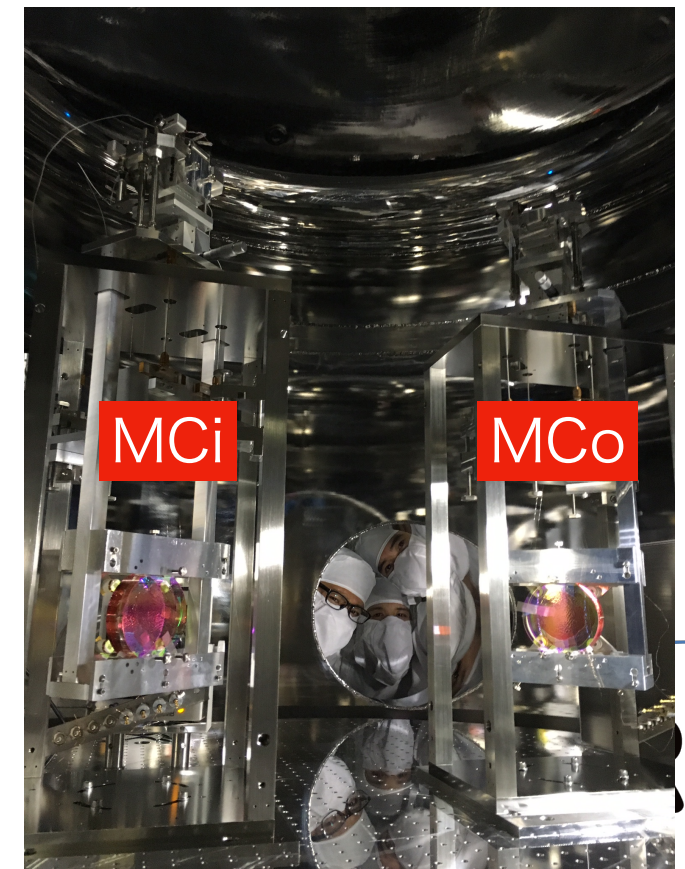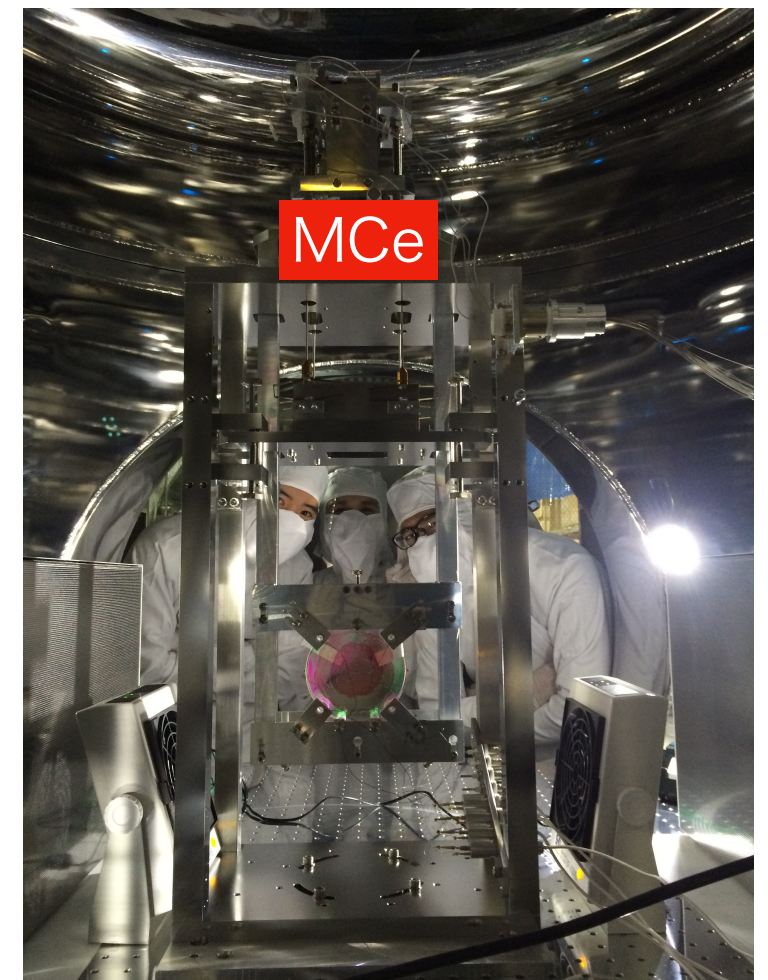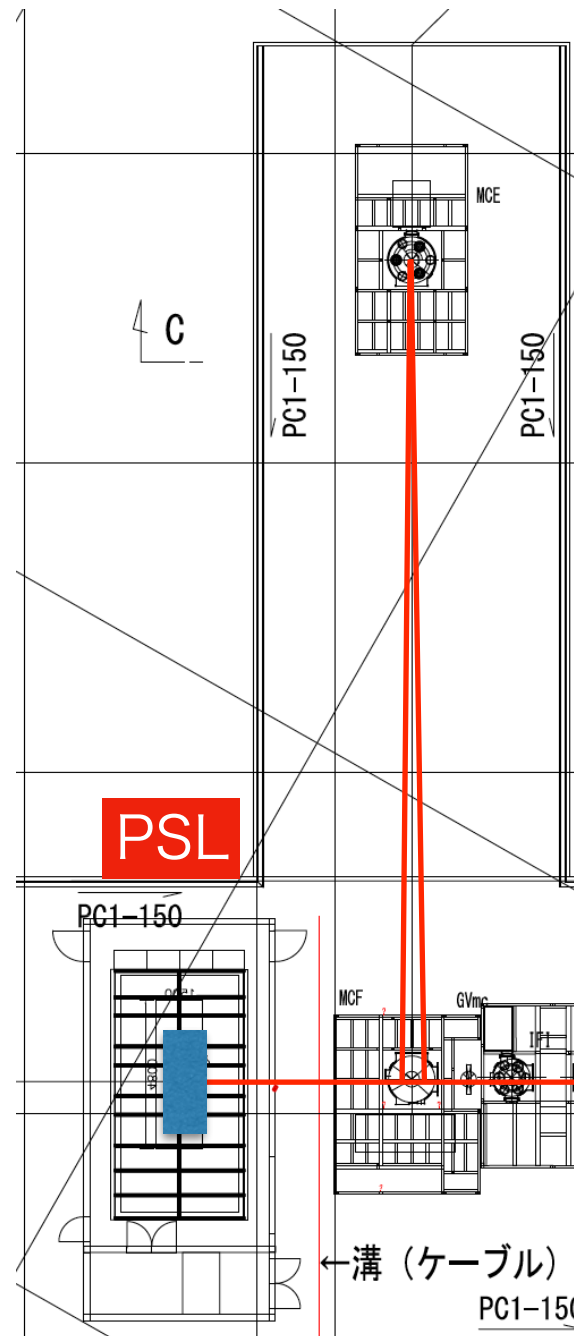

Frequency Noise


- The frequency noise was measured by using the Xarm at the frequencies above ~ 400 Hz
 - ✓ It is consistent with the estimated frequency noise by using the in-loop signals

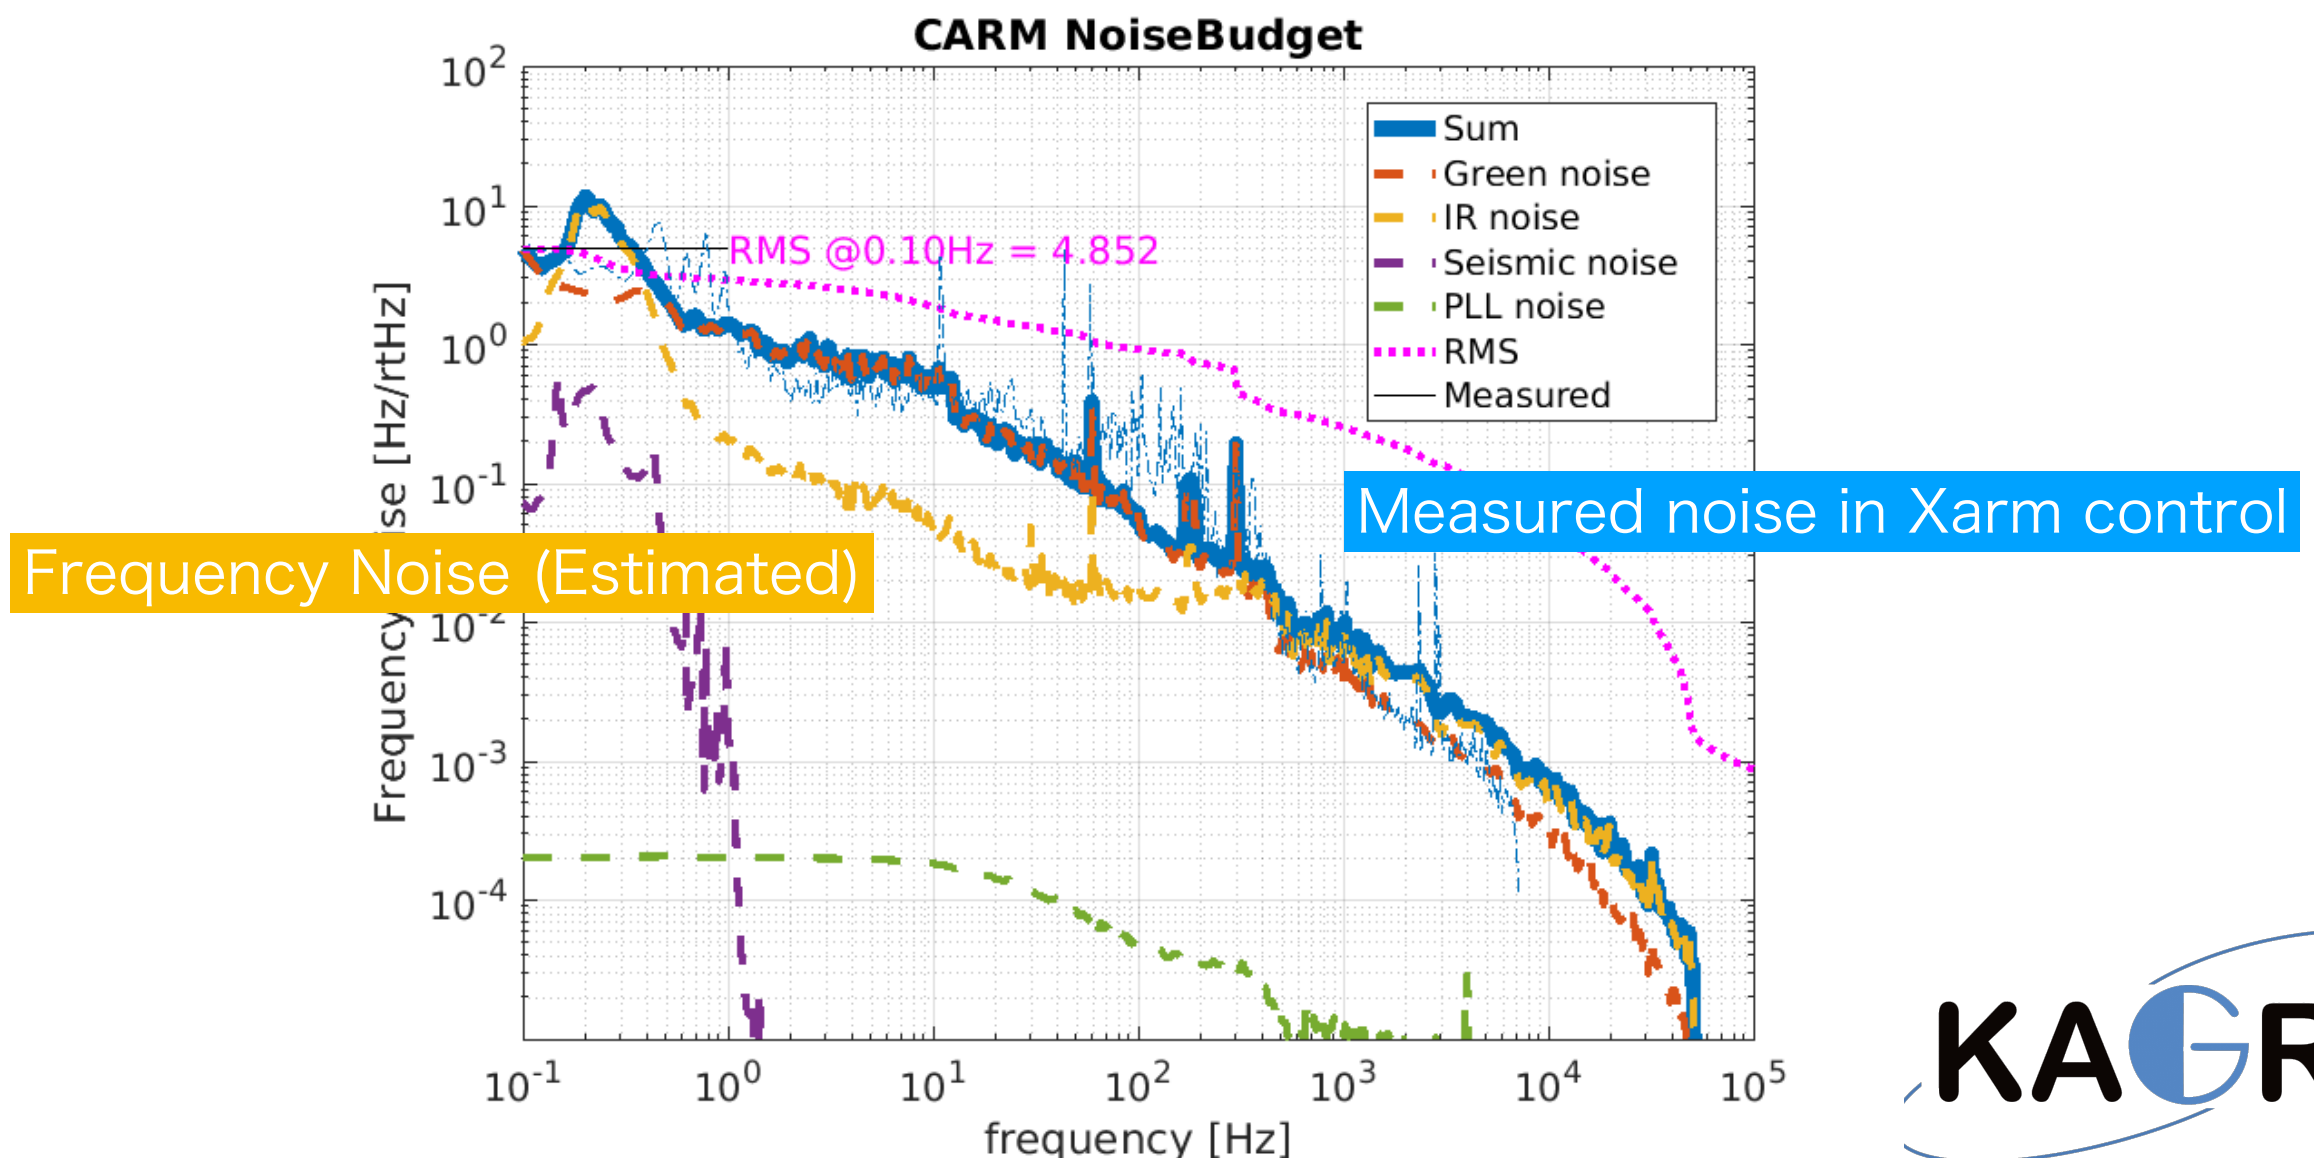


IMC Alignment Sensing and Control (ASC)

IMC alignment sensing & control (ASC)


- 5 sensors
 - ✓ WFS on the IMC REFL table
 - ✓ DC QPD for the MCe TRANS
 - ✓ DC QPD for the IMMT TRANS
- 5 DOFs to be controlled
 - ✓ Cavity axis (3 DOFs for each direction)
 - ➔ The cavity axis determines the output beam axis.
 - ✓ Injection beam (2 DOFs for each direction)
- 5 actuators
 - ✓ Input pointing PZTs.
 - ➔ In the PSL room.
 - ✓ IMC suspended mirrors.

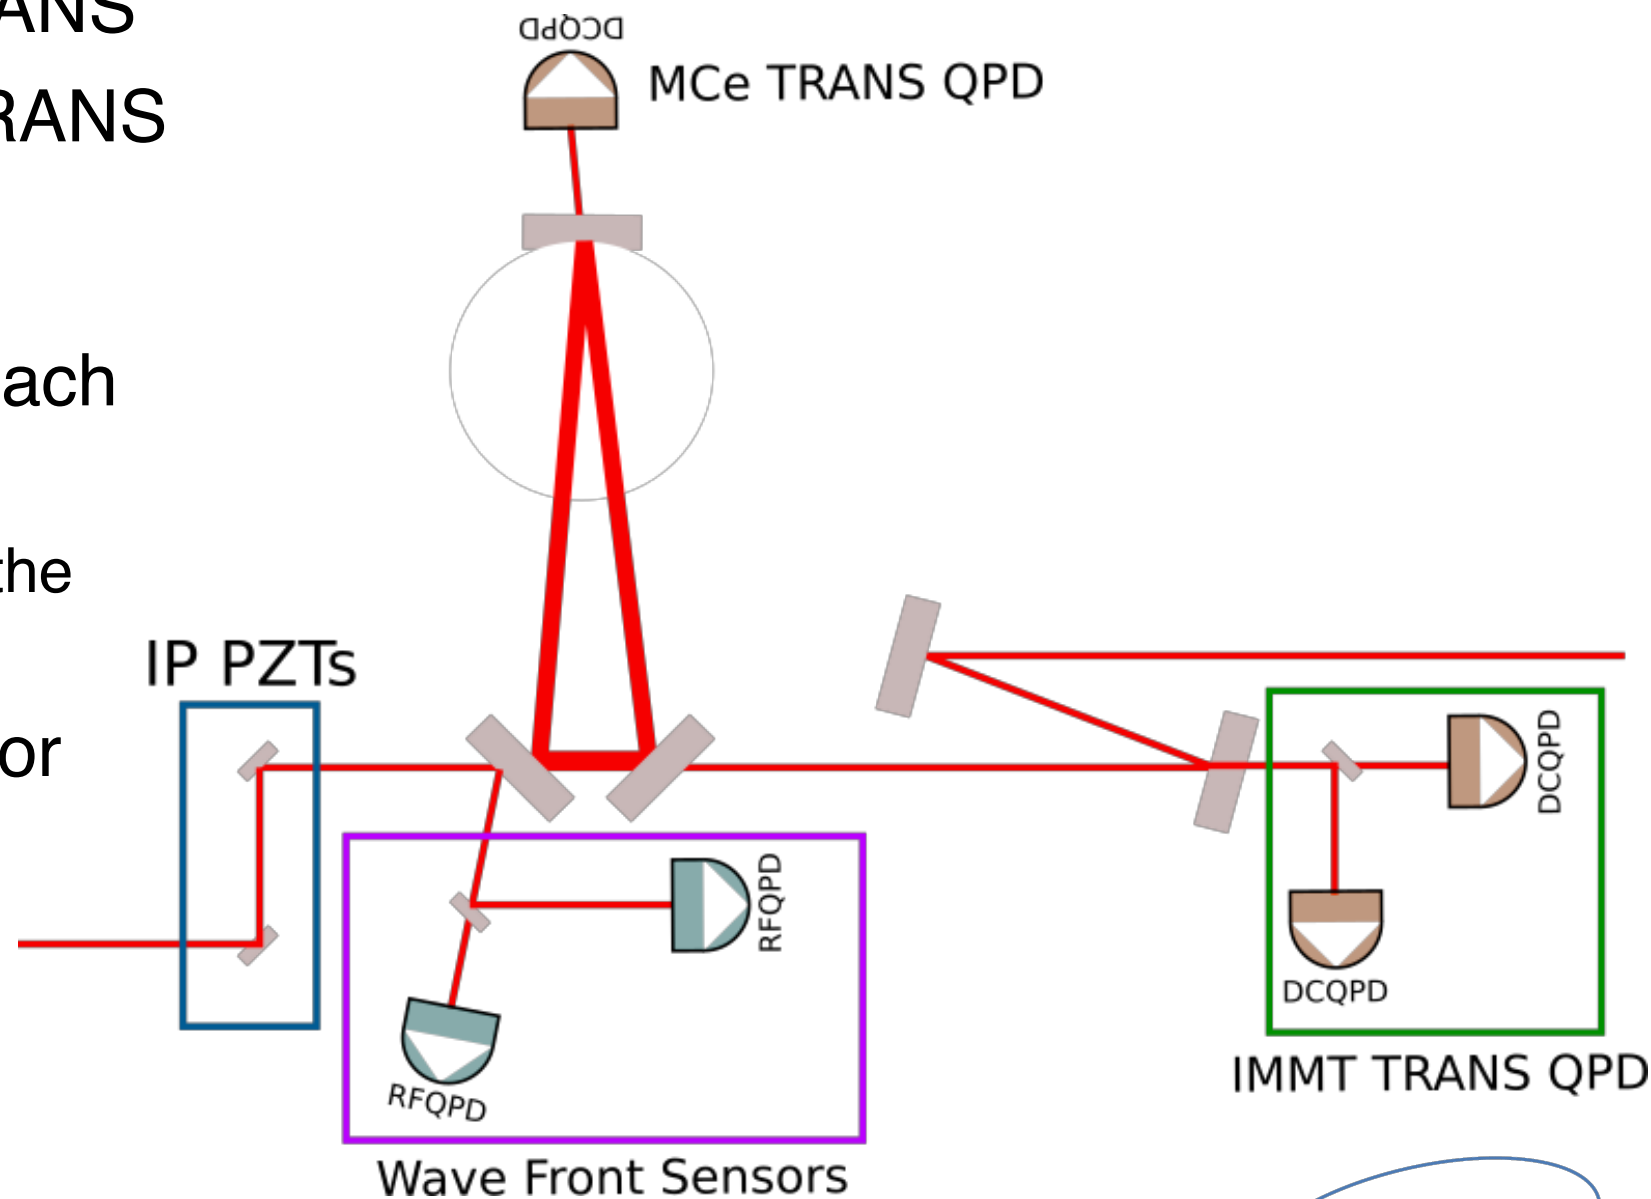


IMC ASC (current configuration)

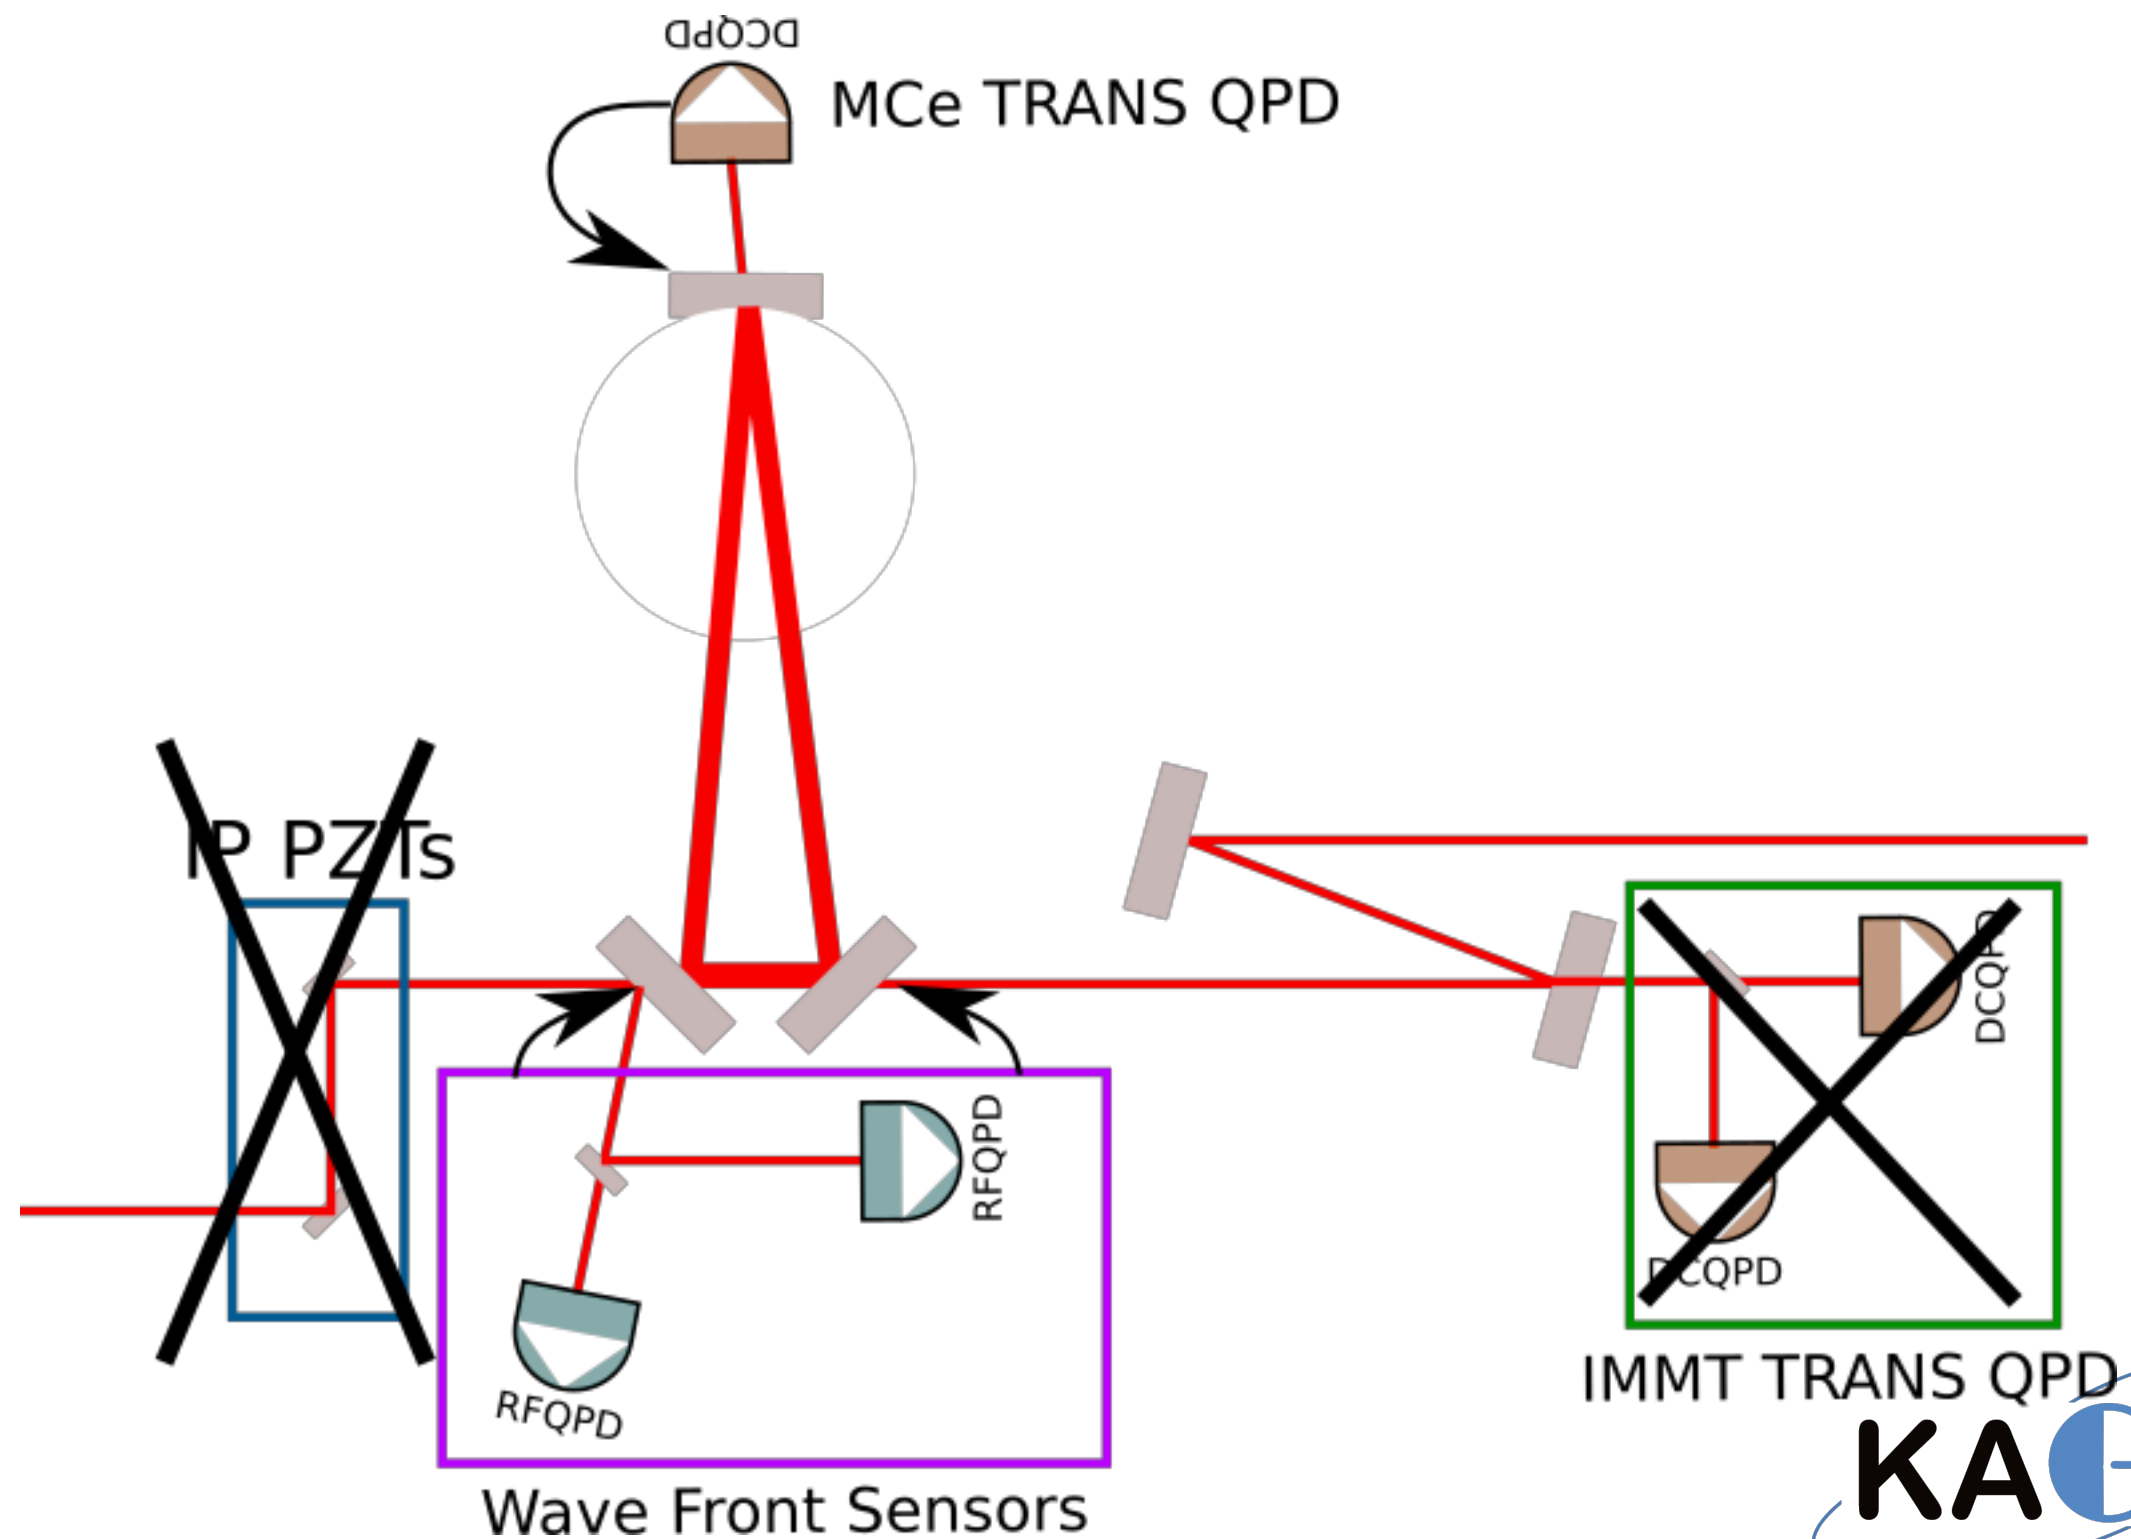

IMC ASC (final configuration 1)

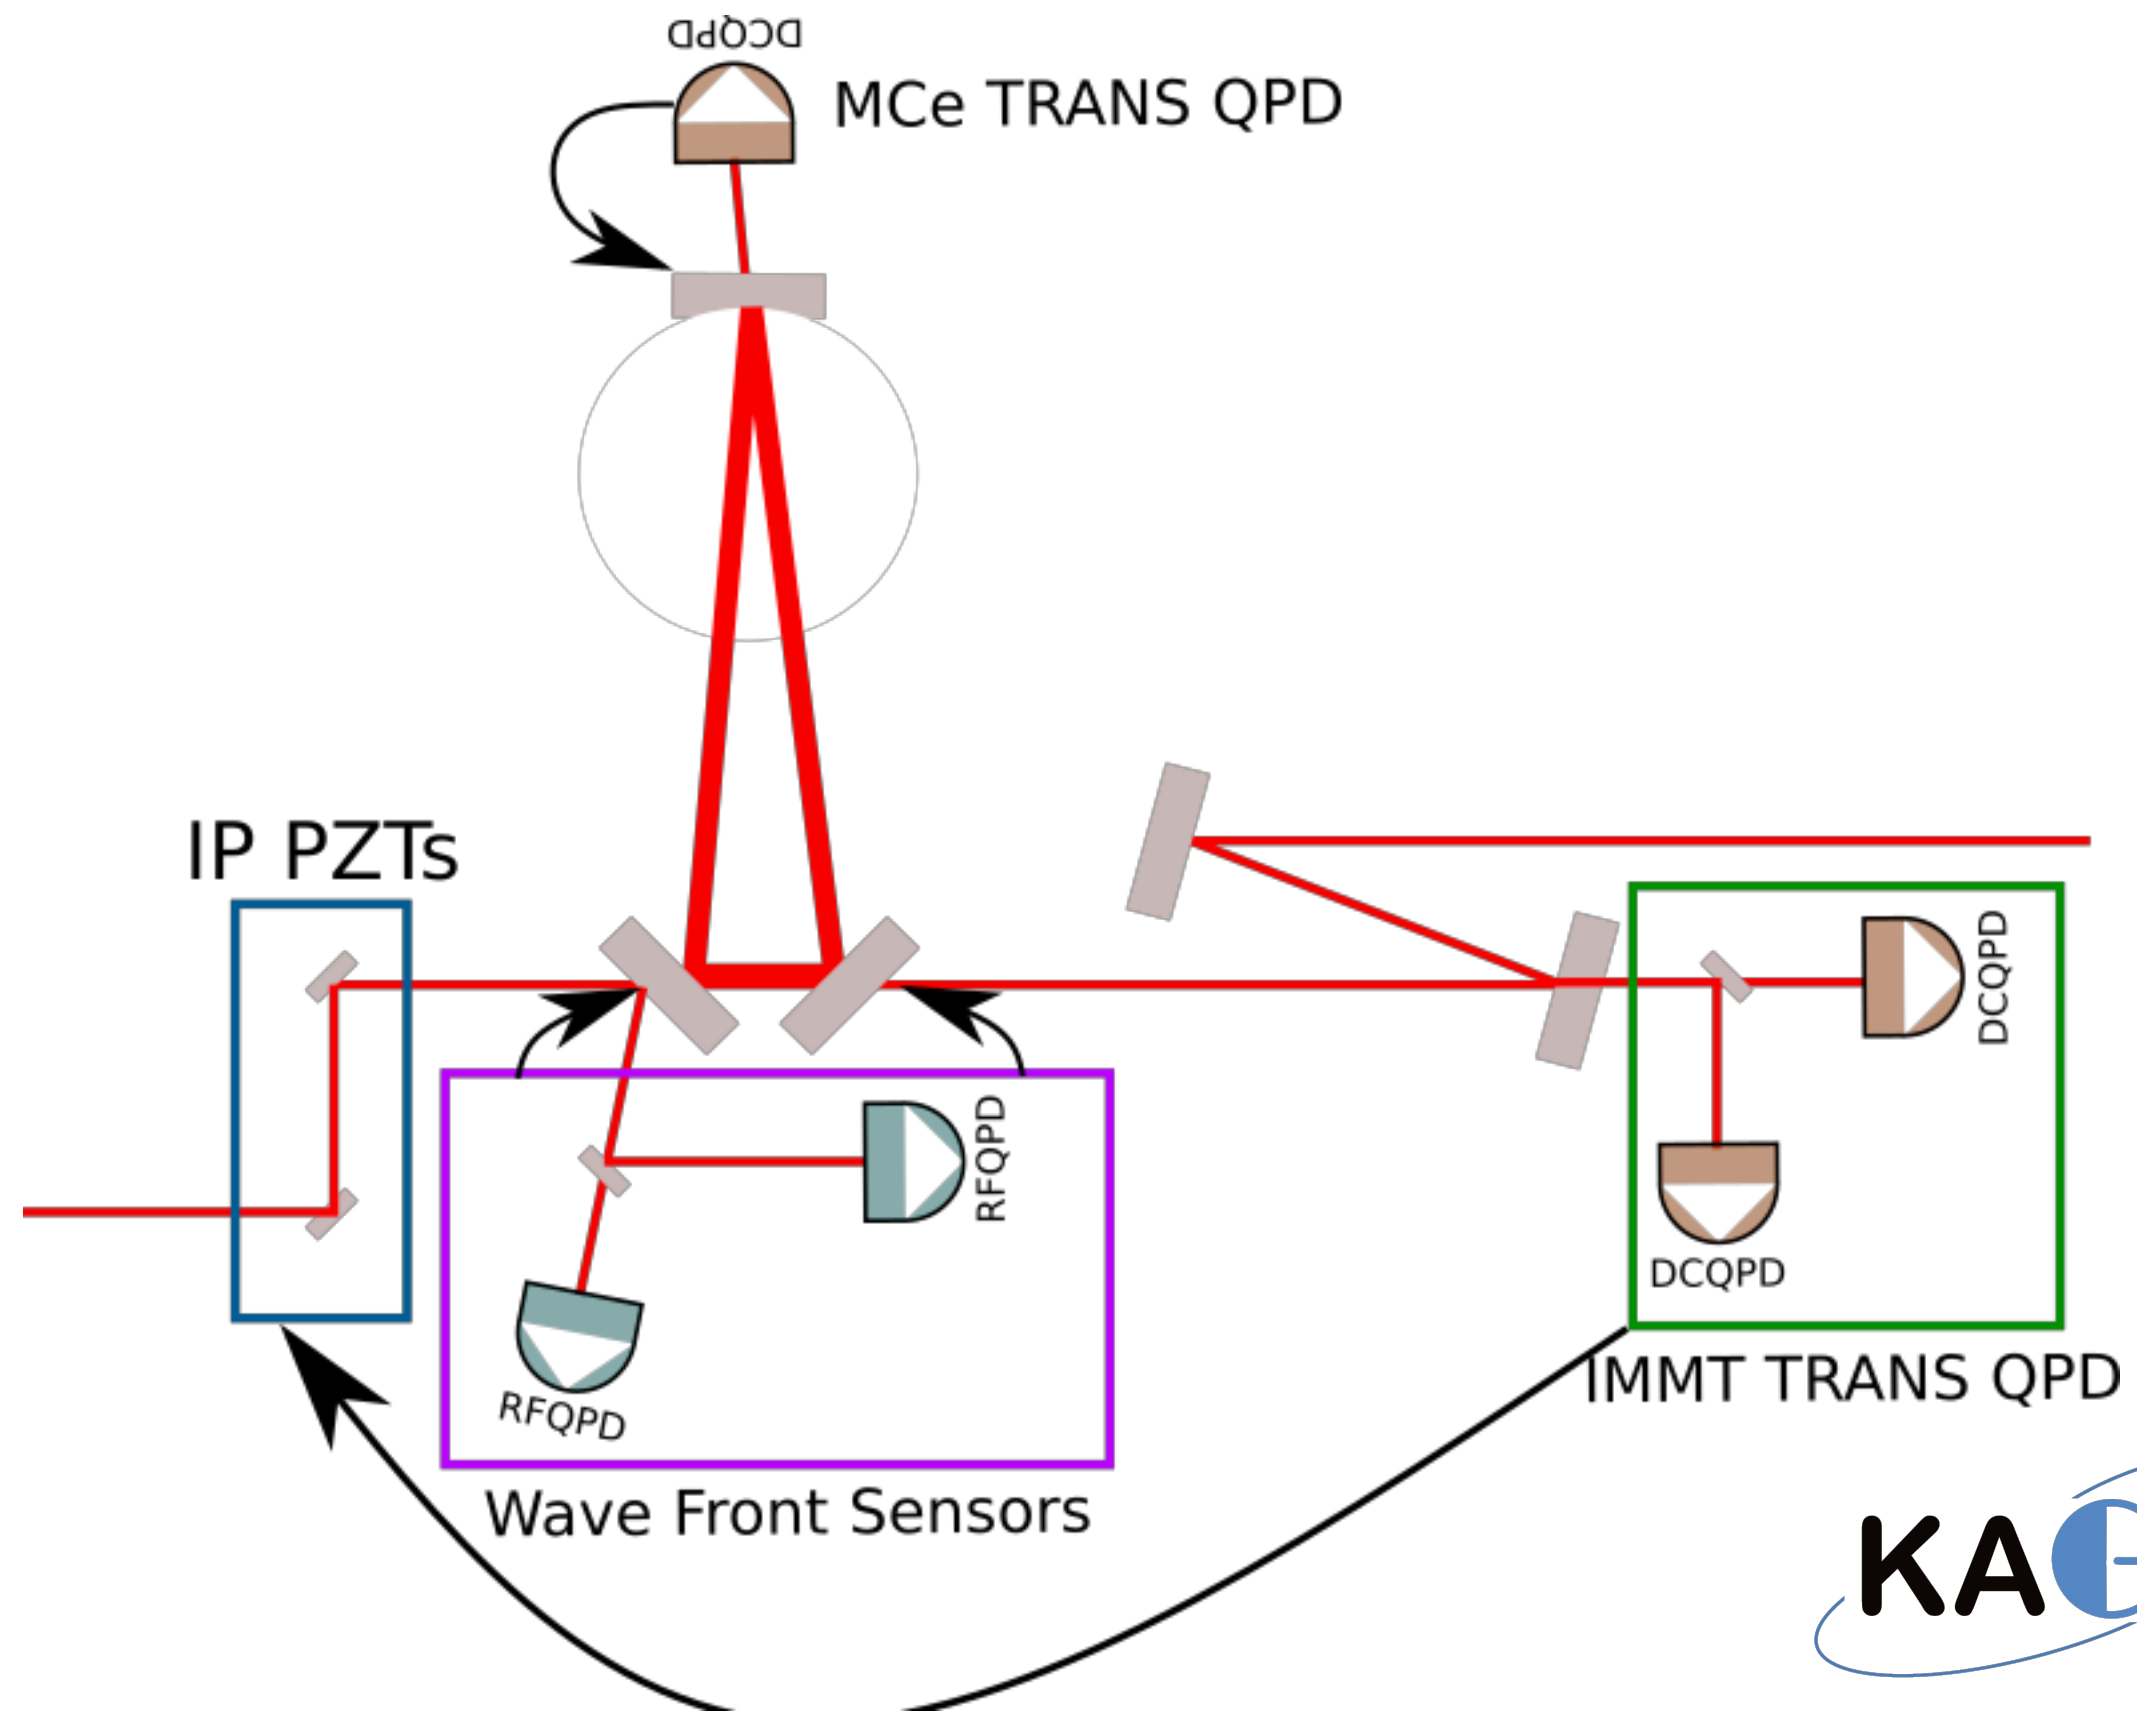


IMC ASC (final configuration 2)

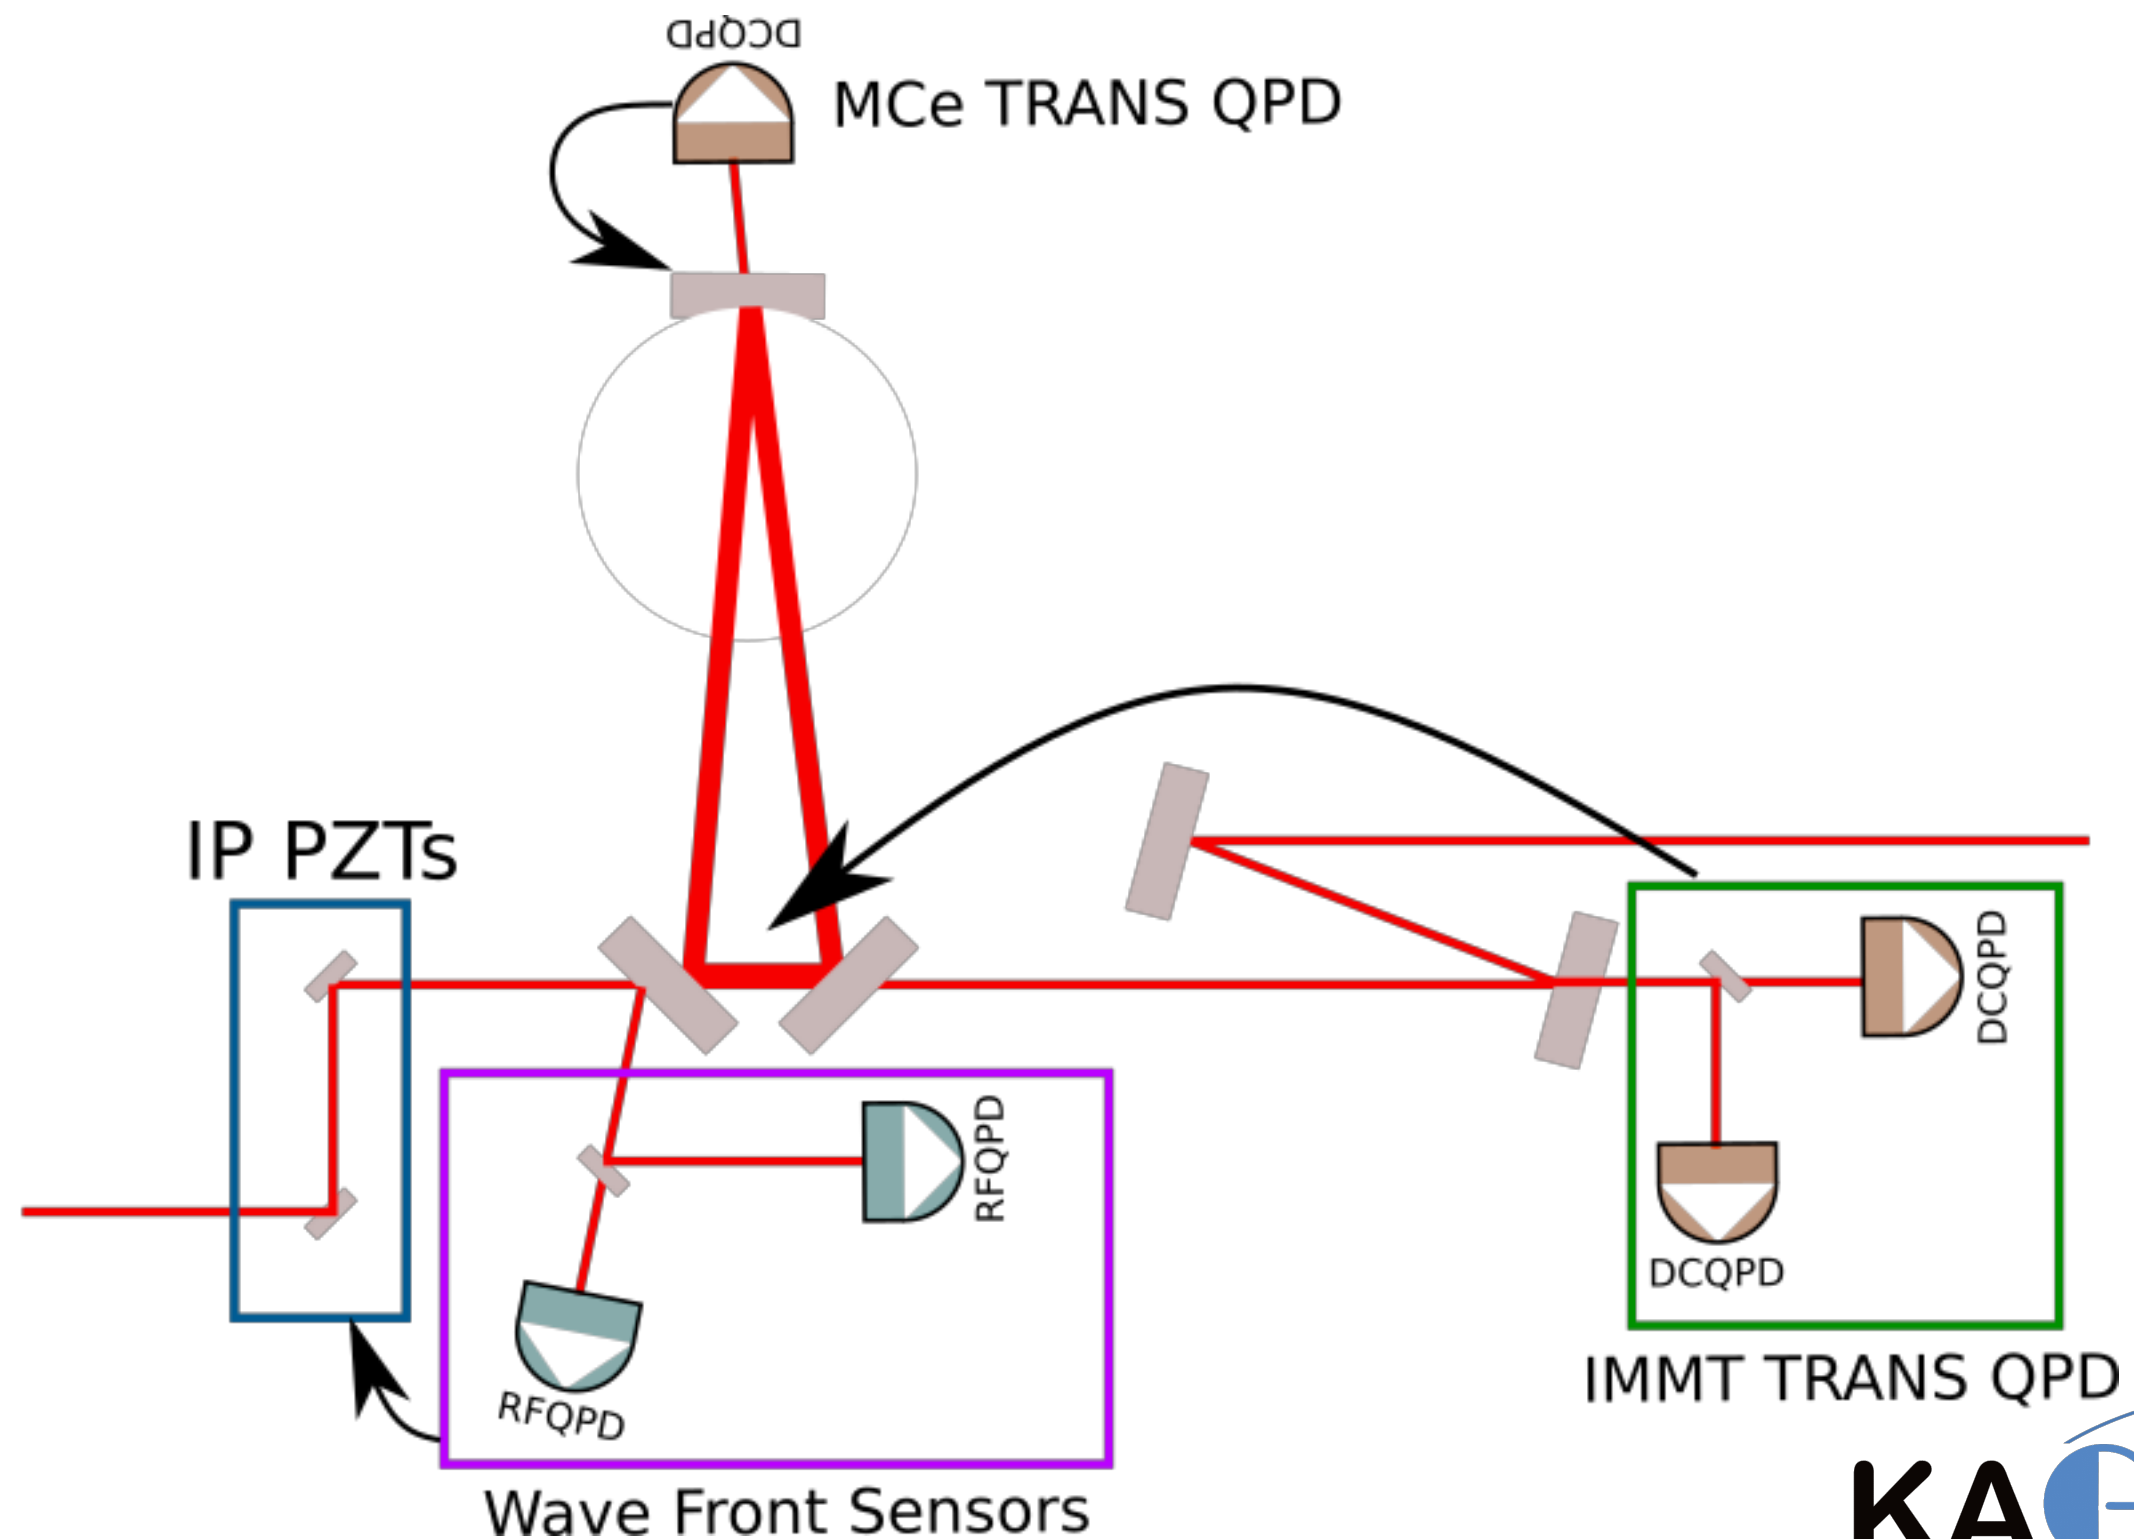

Mach-Zehnder Modulator (MZM)


Mach-Zehnder Modulator (MZM)

- MZM can generate the tunable AM
 - ✓ To cancel the AM generated by the detuning of the RSE interferometer
 - ✓ To generate the AM for the lock acquisition

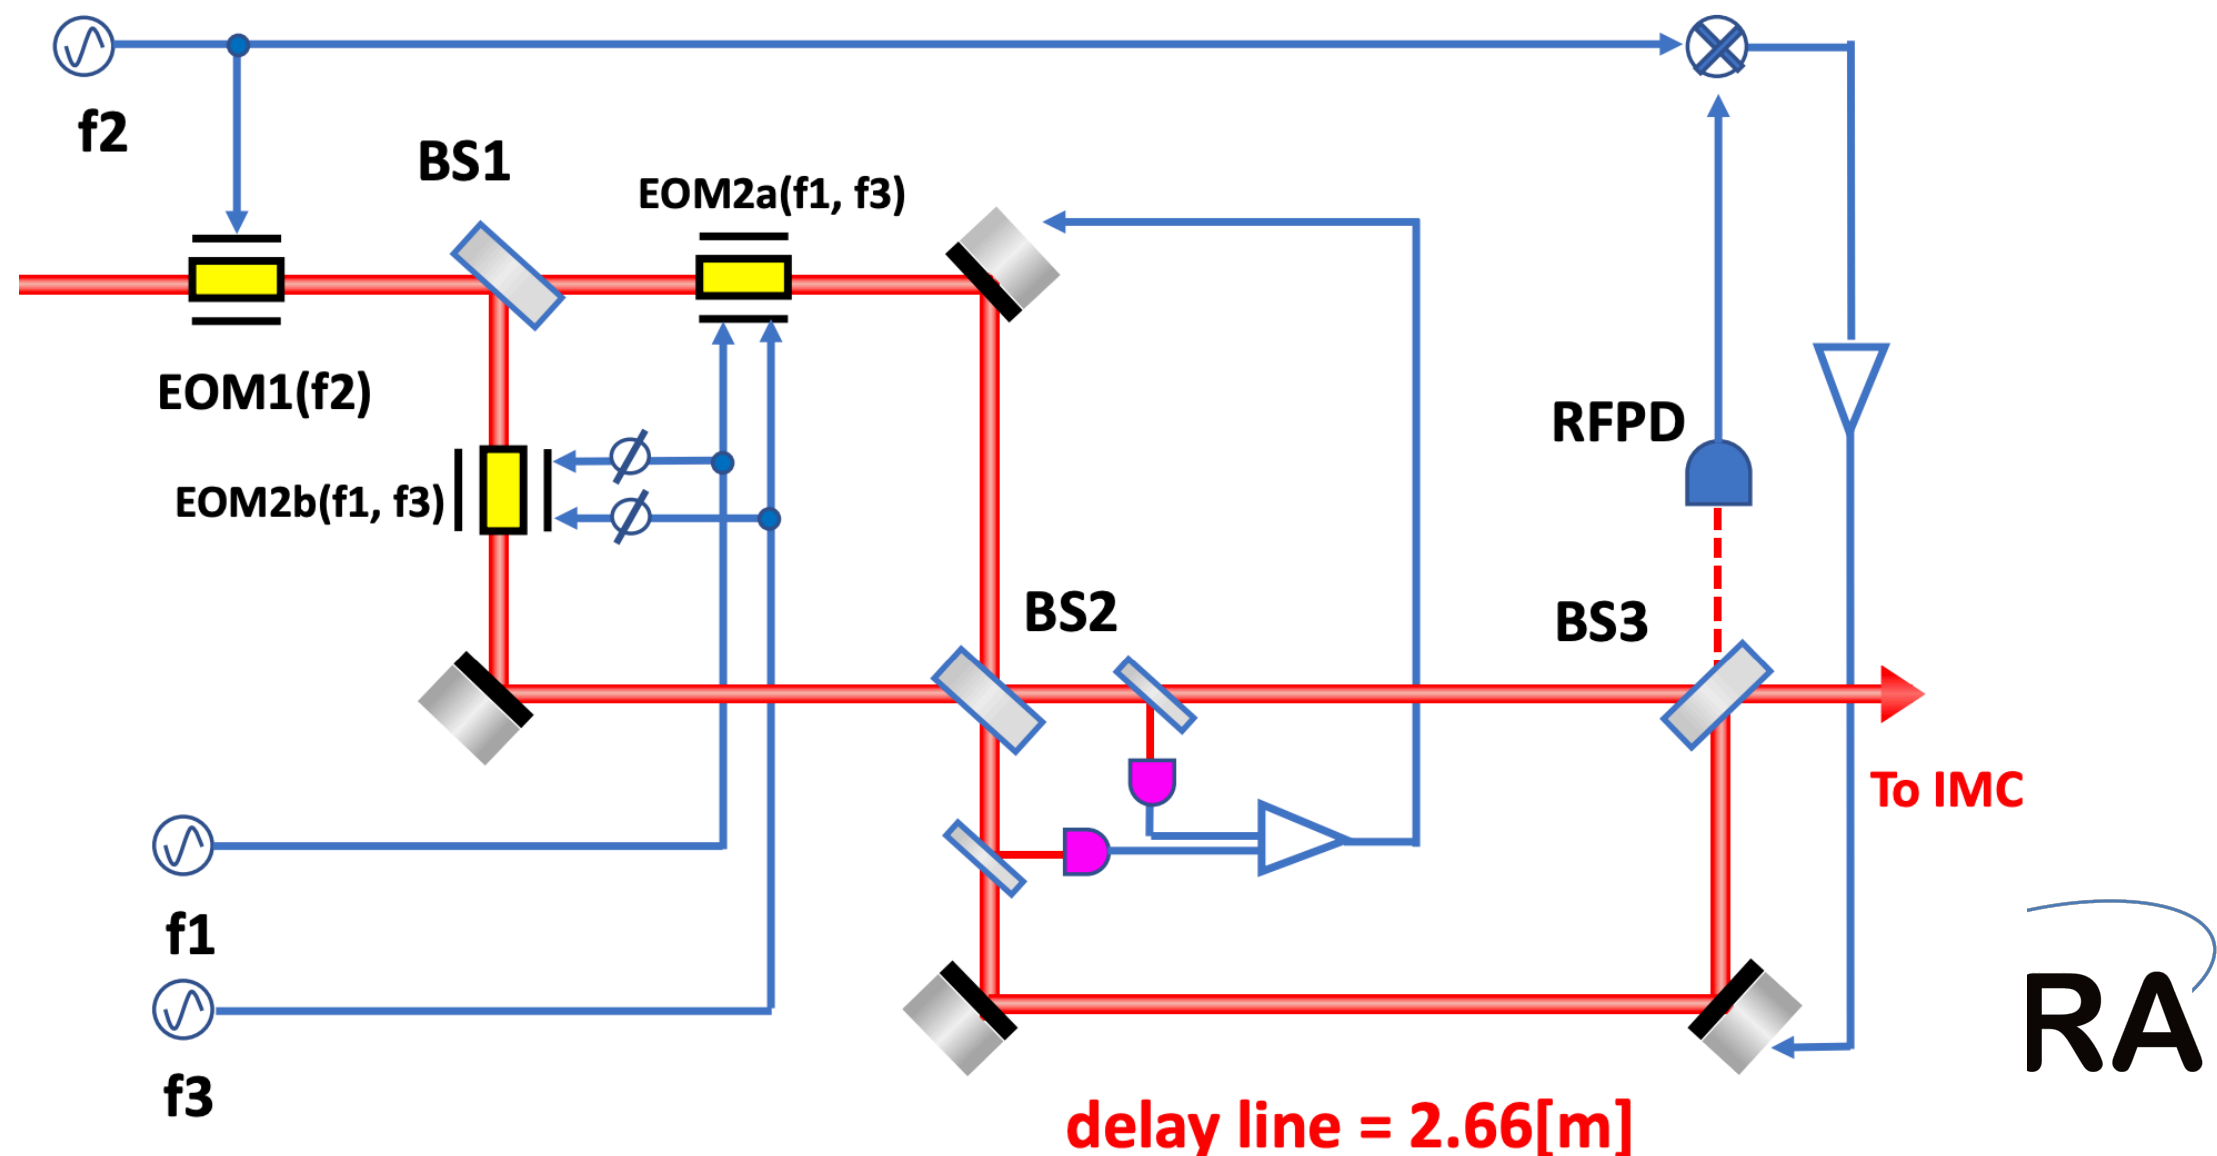


Mach-Zehnder Modulator (MZM)

- The AM can be tuned by tuning the phase difference between the EOMs
 - ✓ Demonstrated by the experiment

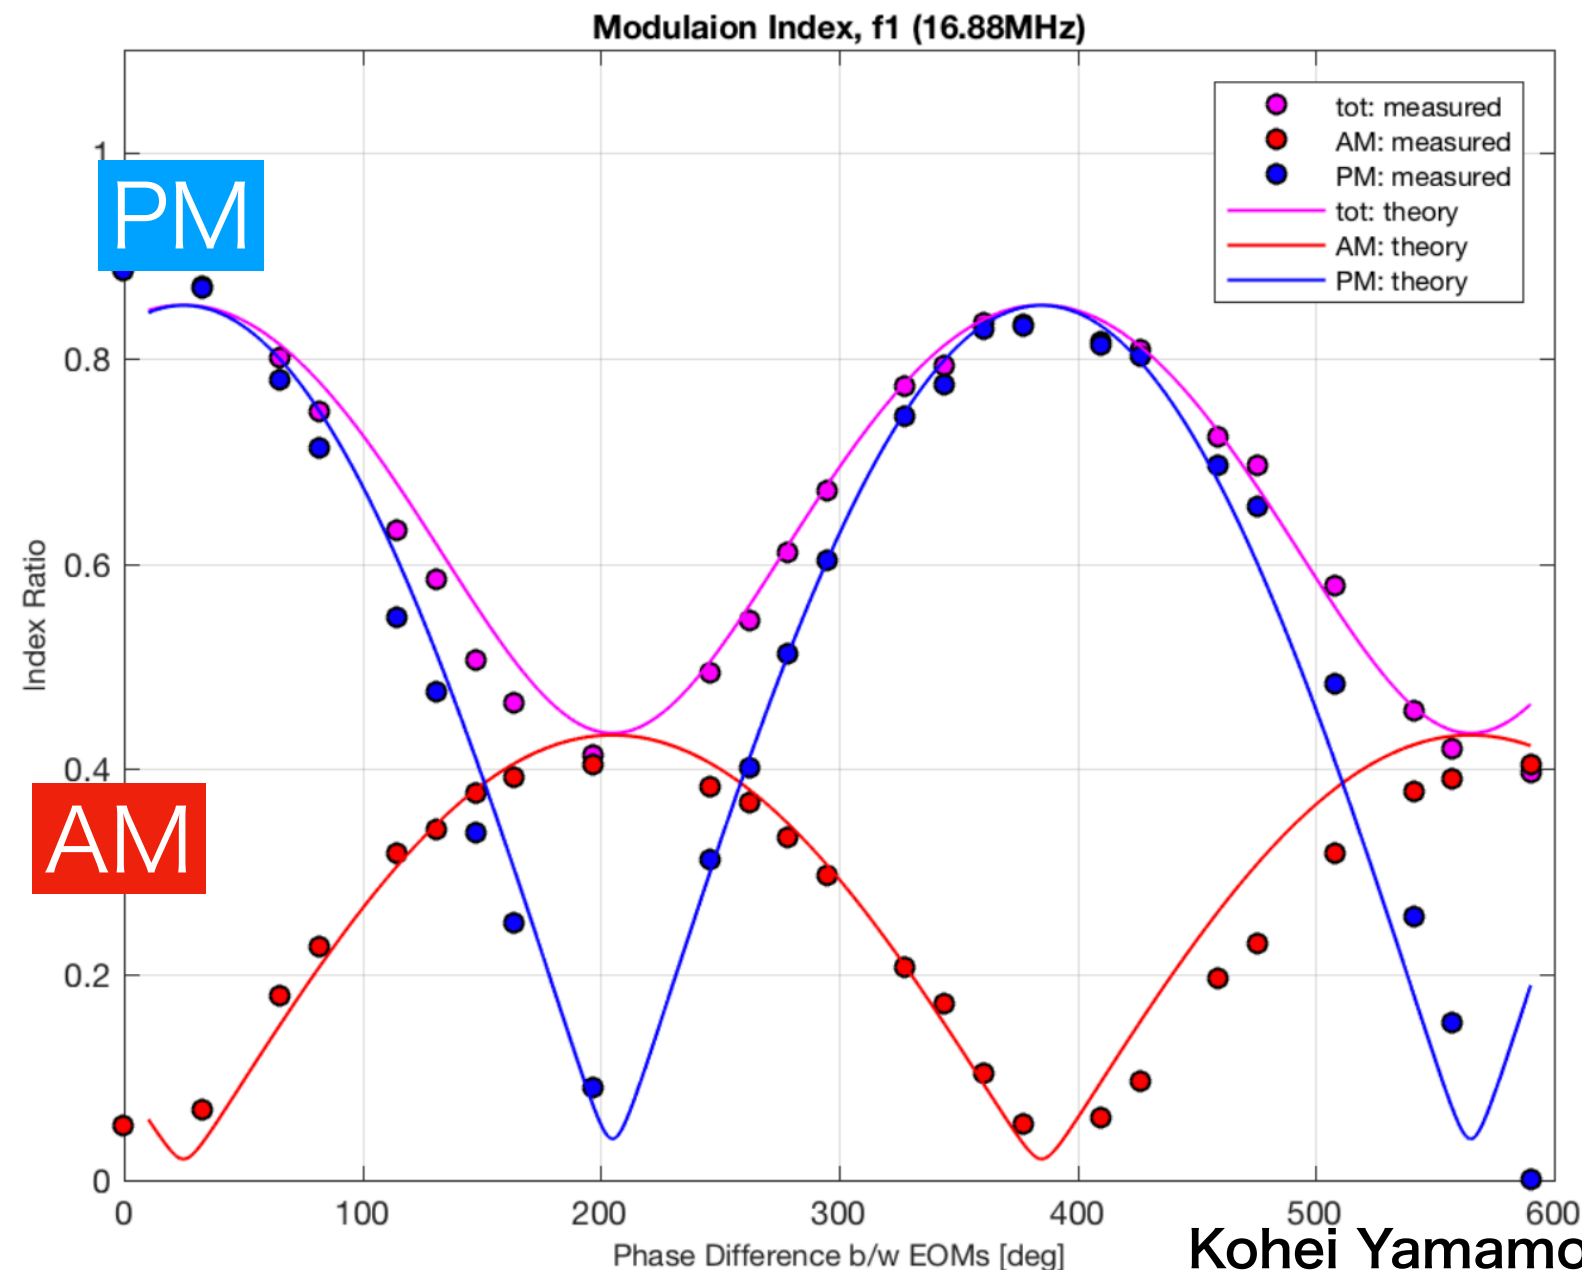

Displacement noise of the MZM


- The displacement noise has not met the requirement

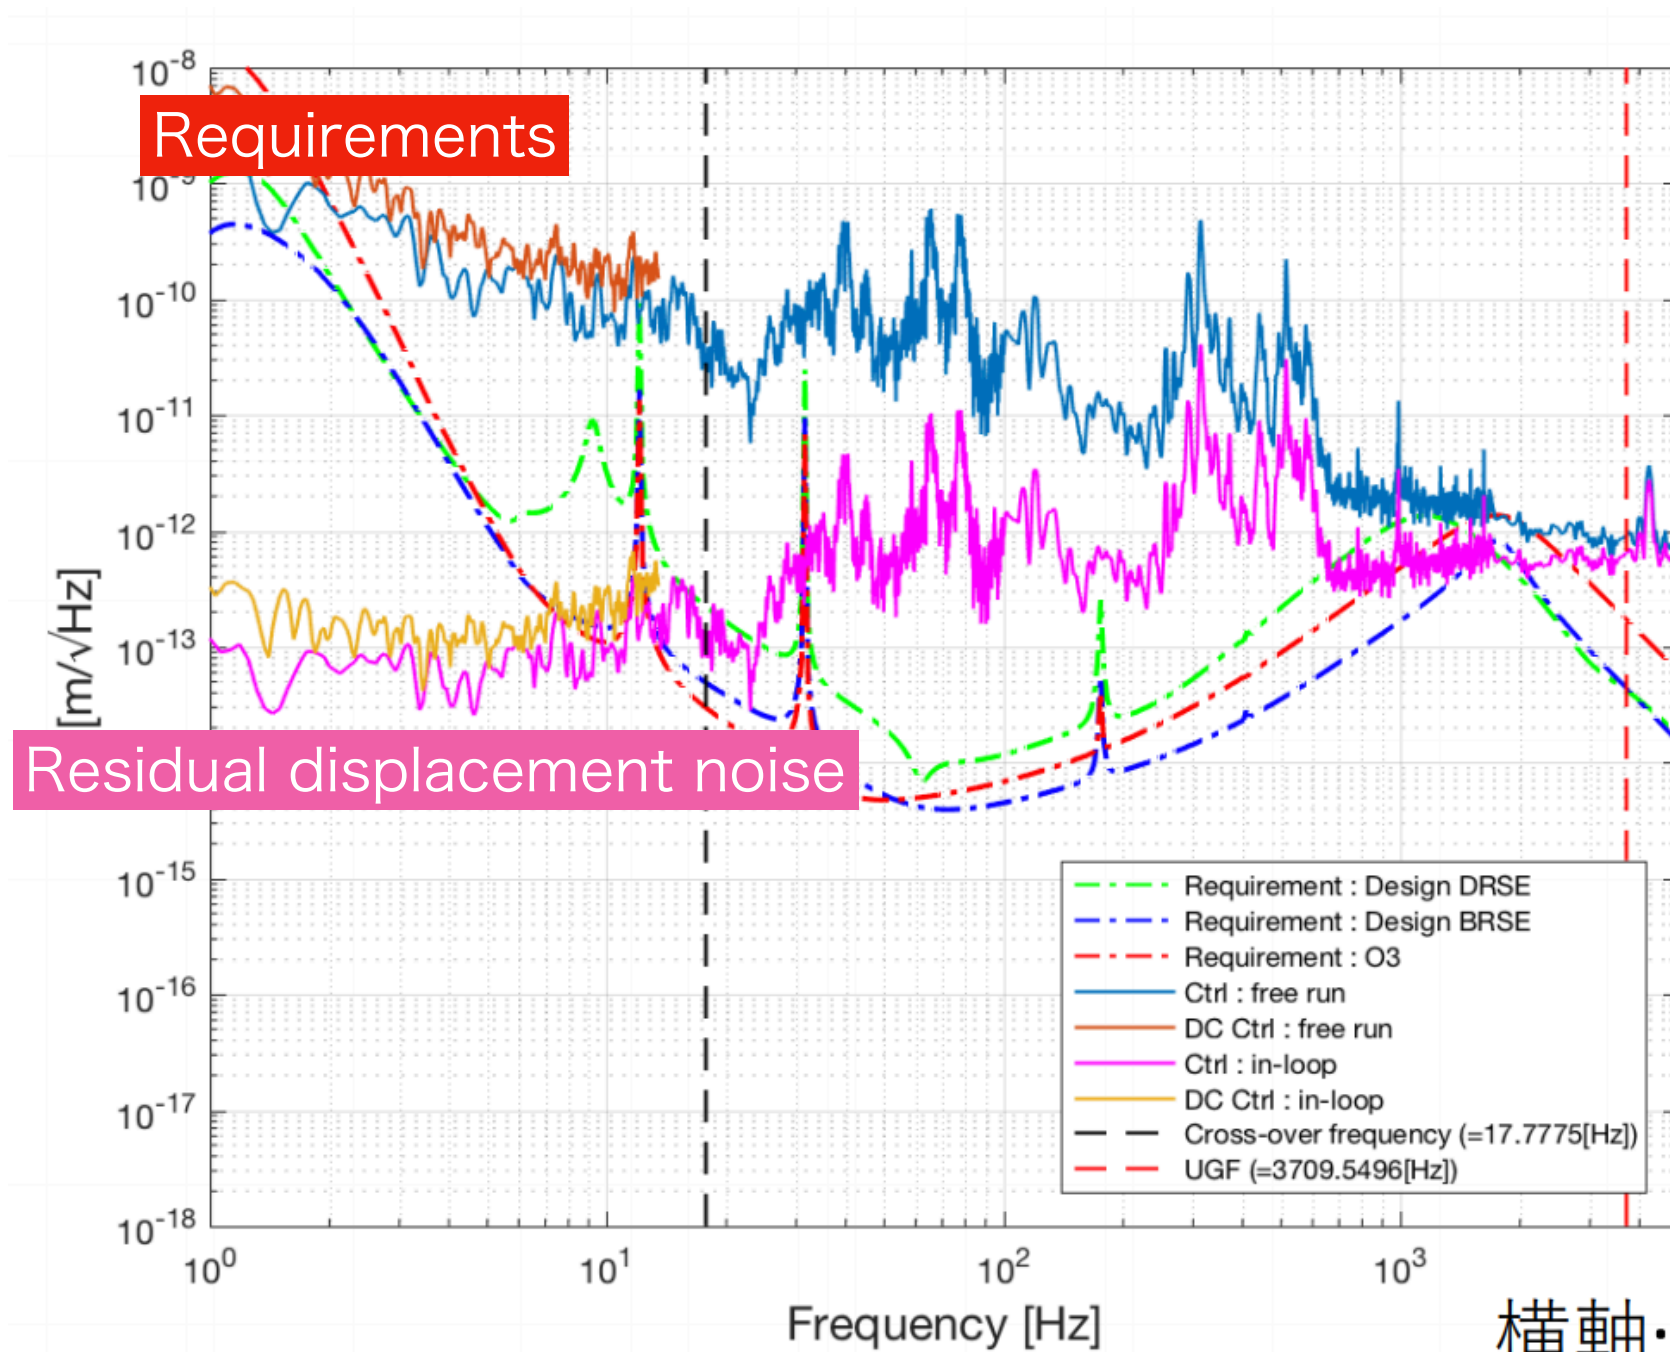

Guardian

Guardian

- All system has been operated automatically by using the guardian.

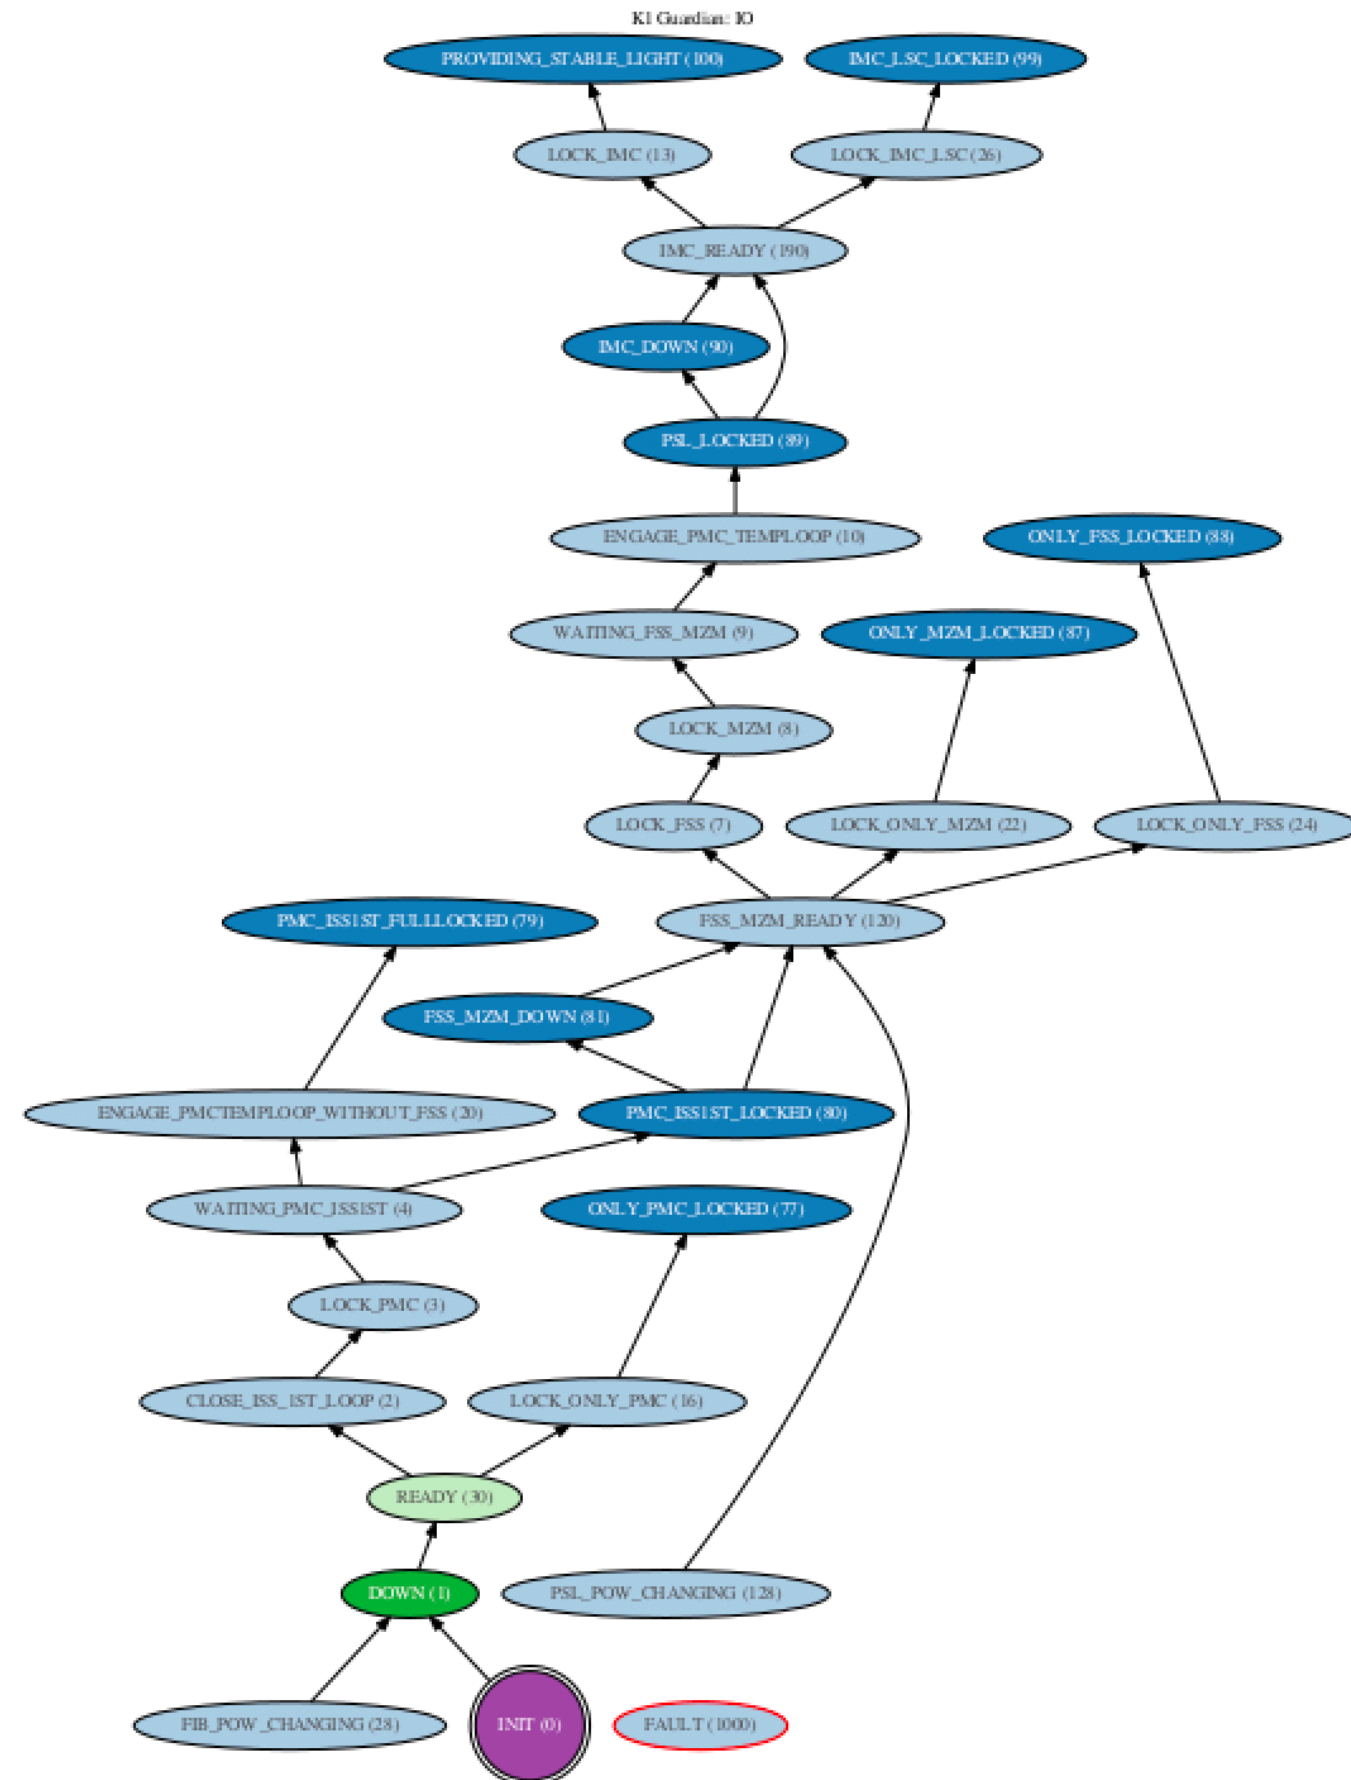

Summary

Summary and future plan

- Almost all system has been installed.
- All system are operated automatically with the guardian.
- The frequency noise has been measured by using the Xarm control signal
 - ✓ It was consistent with the estimation with the in-loop signal.
- IMC ASC is using limited sensors so far.
 - ✓ It will be finalized in a couple of weeks.
- MZM has been installed and demonstrated to generate the tunable AM.
 - ✓ The displacement noise has not met the requirement.
 - Use the monolithic MZI?
 - Use the rigid mirror mounts?
- High power test is on going.

Appendix

Control Bandwidth of the PMC

- UGF: ~ 6 kHz \rightarrow Is enough?

