

*The cooling scenario for O4 without frosting  
on the surface of the KAGRA Test Mass and ....*



Nobuhiro KIMURA

*Institute for Cosmic Ray Research*

*The University of Tokyo*

On behalf of the cryogenic subgroup of KAGRA

2021 Gravitational Wave Advanced Detector Workshop 20/May/2021

# Outline

## ✓ *Introduction*

- *An example of frosting on the surface of view ports*
- *Cryogenic system for KAGRA*
- *Issues in de-frosting experiment using KAGRA cryostat*


## ✓ *Results of de-frosting experiment using KAGRA cryostat*

- *Test mass cooling by the scenario for O4*
- *Residual gas measurement during the Test Mass cooling*
- *Performance defrost heaters*

## ✓ *Summaries*


## *An example of frosting on the surface of view port*

- Frosting on the surface of the test mass and the viewports of the radiation shields is a serious problem at the KAGRA.
- In order to find a way to cool the test mass down to  $\sim 20$  K while preventing frosting, KAGRA cryogenic subgroup have conducted the cooling experiment using the KAGRA cryostat.

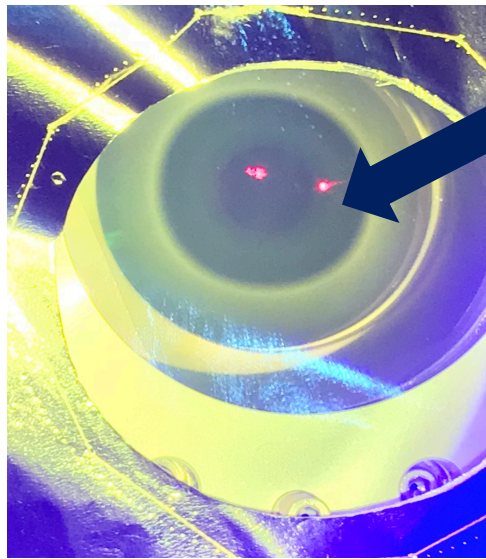

TM oplev light source side

*Frosting*

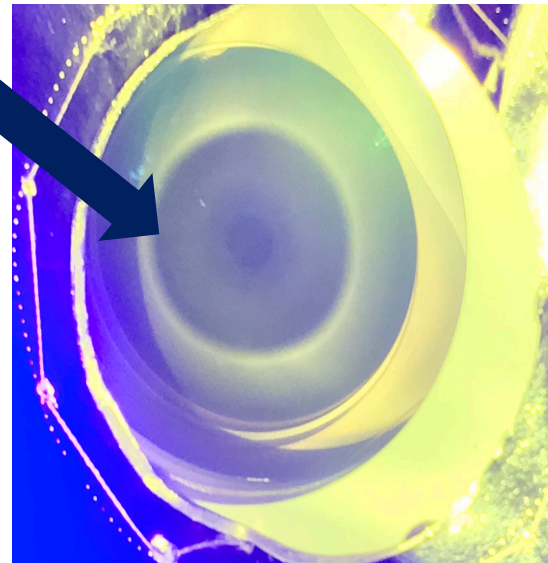


TM oplev QPD side

Photos show examples of the frosting on the surface of view ports with vacuum leak at TM temperature of  $\sim 25$  K. (@EXC 2020/08)


It was assumed that frog on the surface was formed by frosting of  $O_2$ ,  $N_2$  and  $H_2O$ .

# Structural view of KAGRA Cryostat with shield ducts

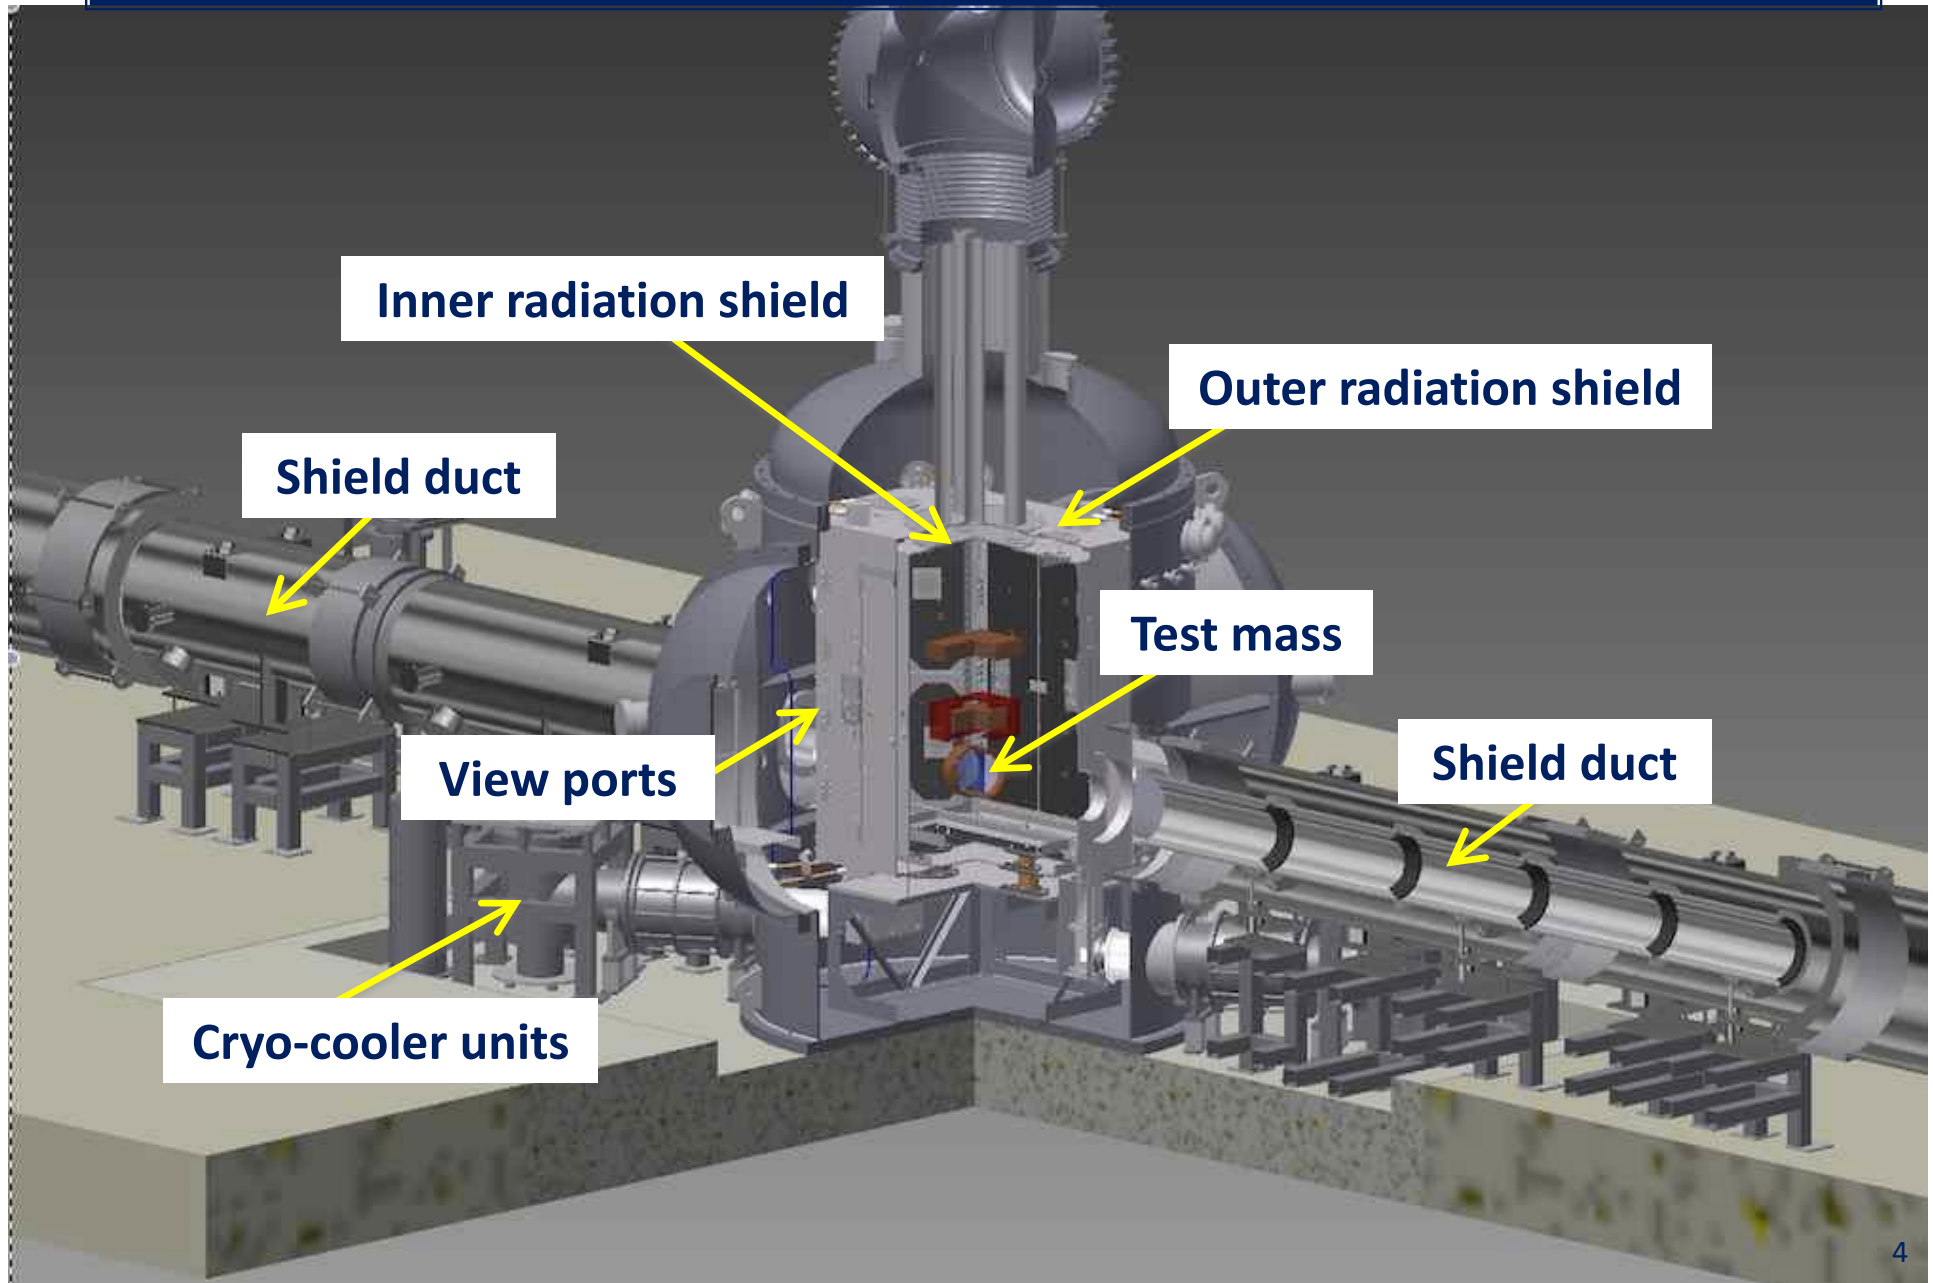

# Cryo-cooler layout

Pulse Tube type Cryo-cooler (PTC) with Vibration reduction

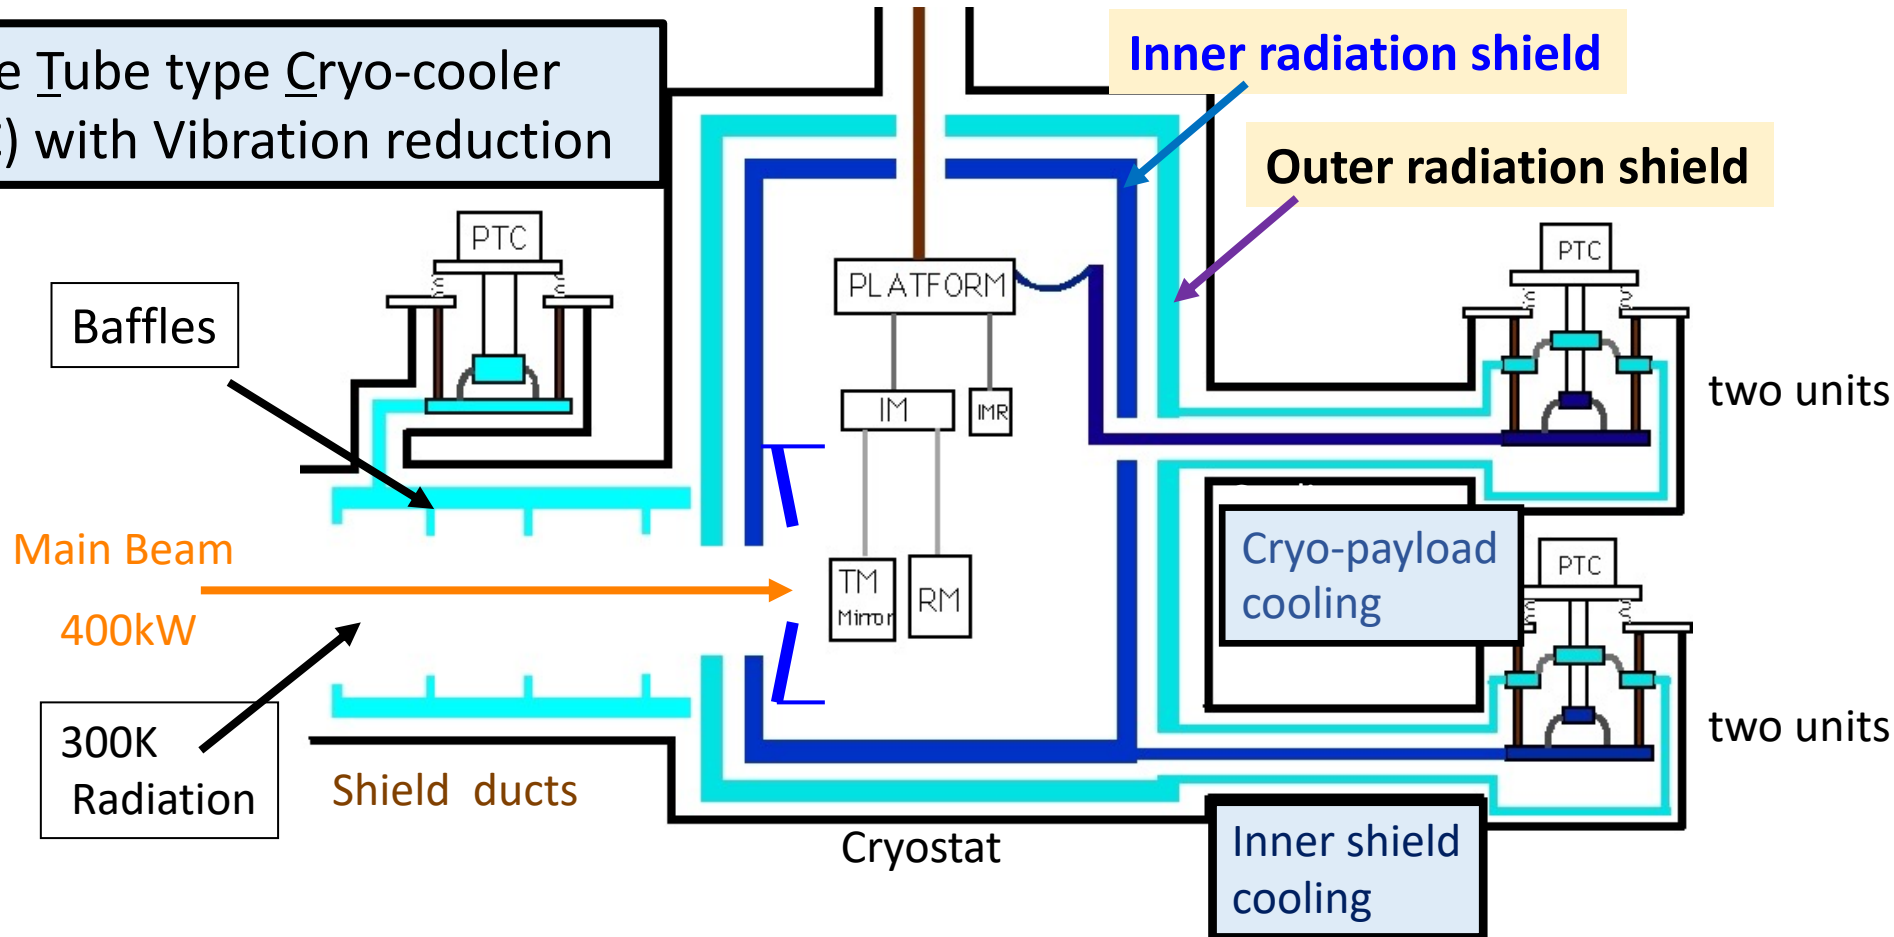

- Four 4K cryocooler units per one cryostat

→ { 2 units for cool cryo-payload  
2 units cool for the inner shield  
4 units cool for the outer shield

# Issues in de-frosting experiment using KAGRA cryostat

## 1. Determine the cooling scheme for Test Mass without frosting

Including confirmation of the occurrence of frosting on the view ports under the condition of leak rate  $<10^{-10}\text{Pam}^{-3}/\text{s}$ )

## 2. Defrosting experiment by defrost heaters

Confirmation of defrost heater performances

(If no frost adheres, check the temperature profile of defrost heating.)

## 3. Measurement of partial pressure of residual gas to confirm frosting components

## Proposed Test mass cooling scenario for O4

- Issue: How maintain mirror temperature lower than 100 K without frosting on the surface of the mirror -

Cooling steps at this experiment;

Step 1:

Start vacuum pumps and wait inner pressure shall be lower than  $\sim 10^{-4}$  Pa.

It will take **21 days** including vacuum leak test for 3 days.

Step 2:

To trap H<sub>2</sub>O residual gas on the surface of duct shield, Start duct shield cryocoolers and wait surface temperature of duct shield shall be lower than lower than  $\sim 150$  K.

It will take **11 days**.

Step 3:

To trap nitrogen gas on the surface of inner shield, start two shield cryocooler units. The mirror is cooled by only radiation to the inner shield.

Wait surface temperature of inner shield shall be lower than lower than  $\sim 20$  K.


It will take **24 days** after switched on the coolers.

Step 4:

Switched on payload cryo-coolers.

It will take **10 days** after switched on the coolers to reach steady state condition of mirror temperature.

# Temperature distribution and pressure in the KAGRA Cryostat after cooling

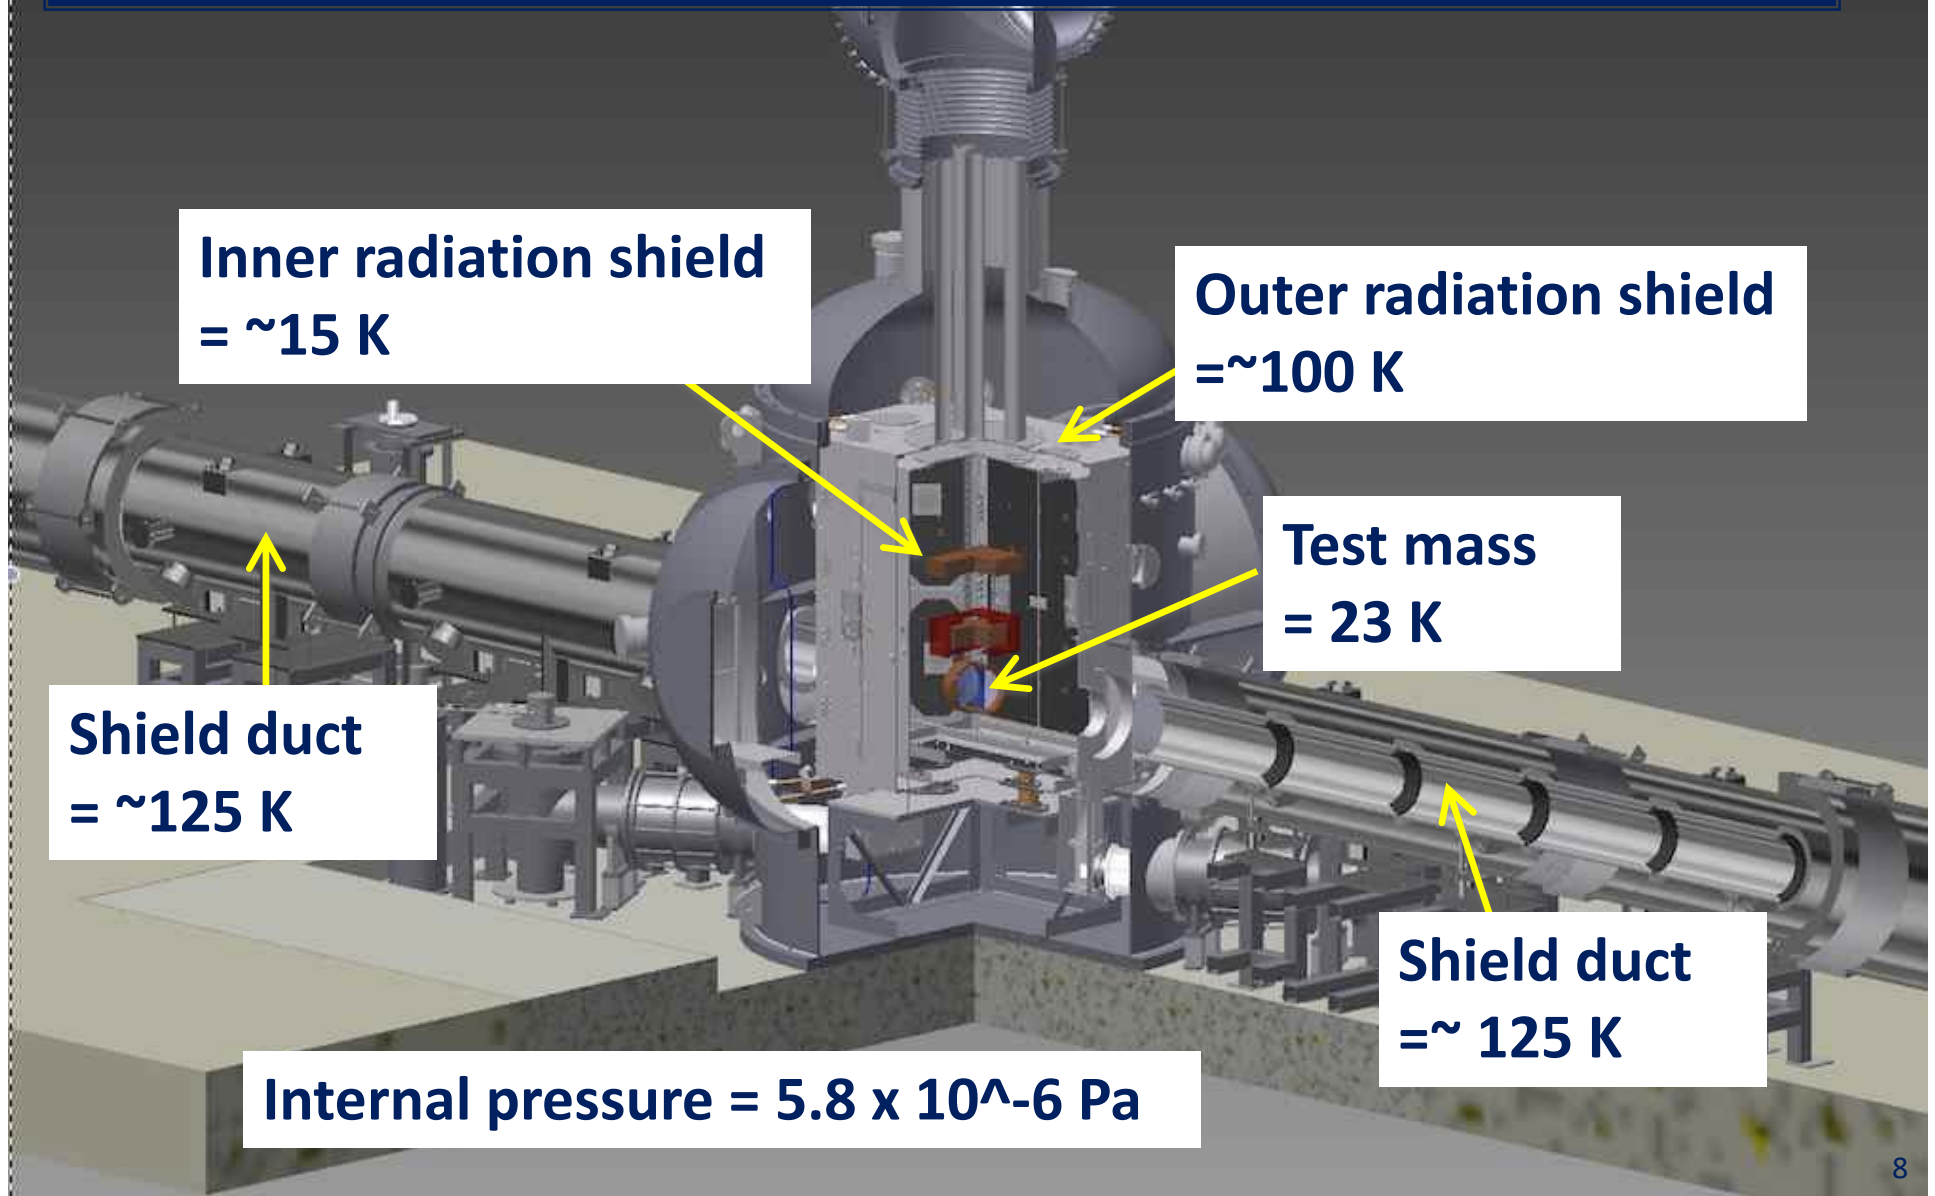

Inner radiation shield  
= ~15 K

Outer radiation shield  
= ~100 K


Test mass  
= 23 K

Shield duct  
= ~125 K


Shield duct  
= ~ 125 K

Internal pressure =  $5.8 \times 10^{-6}$  Pa



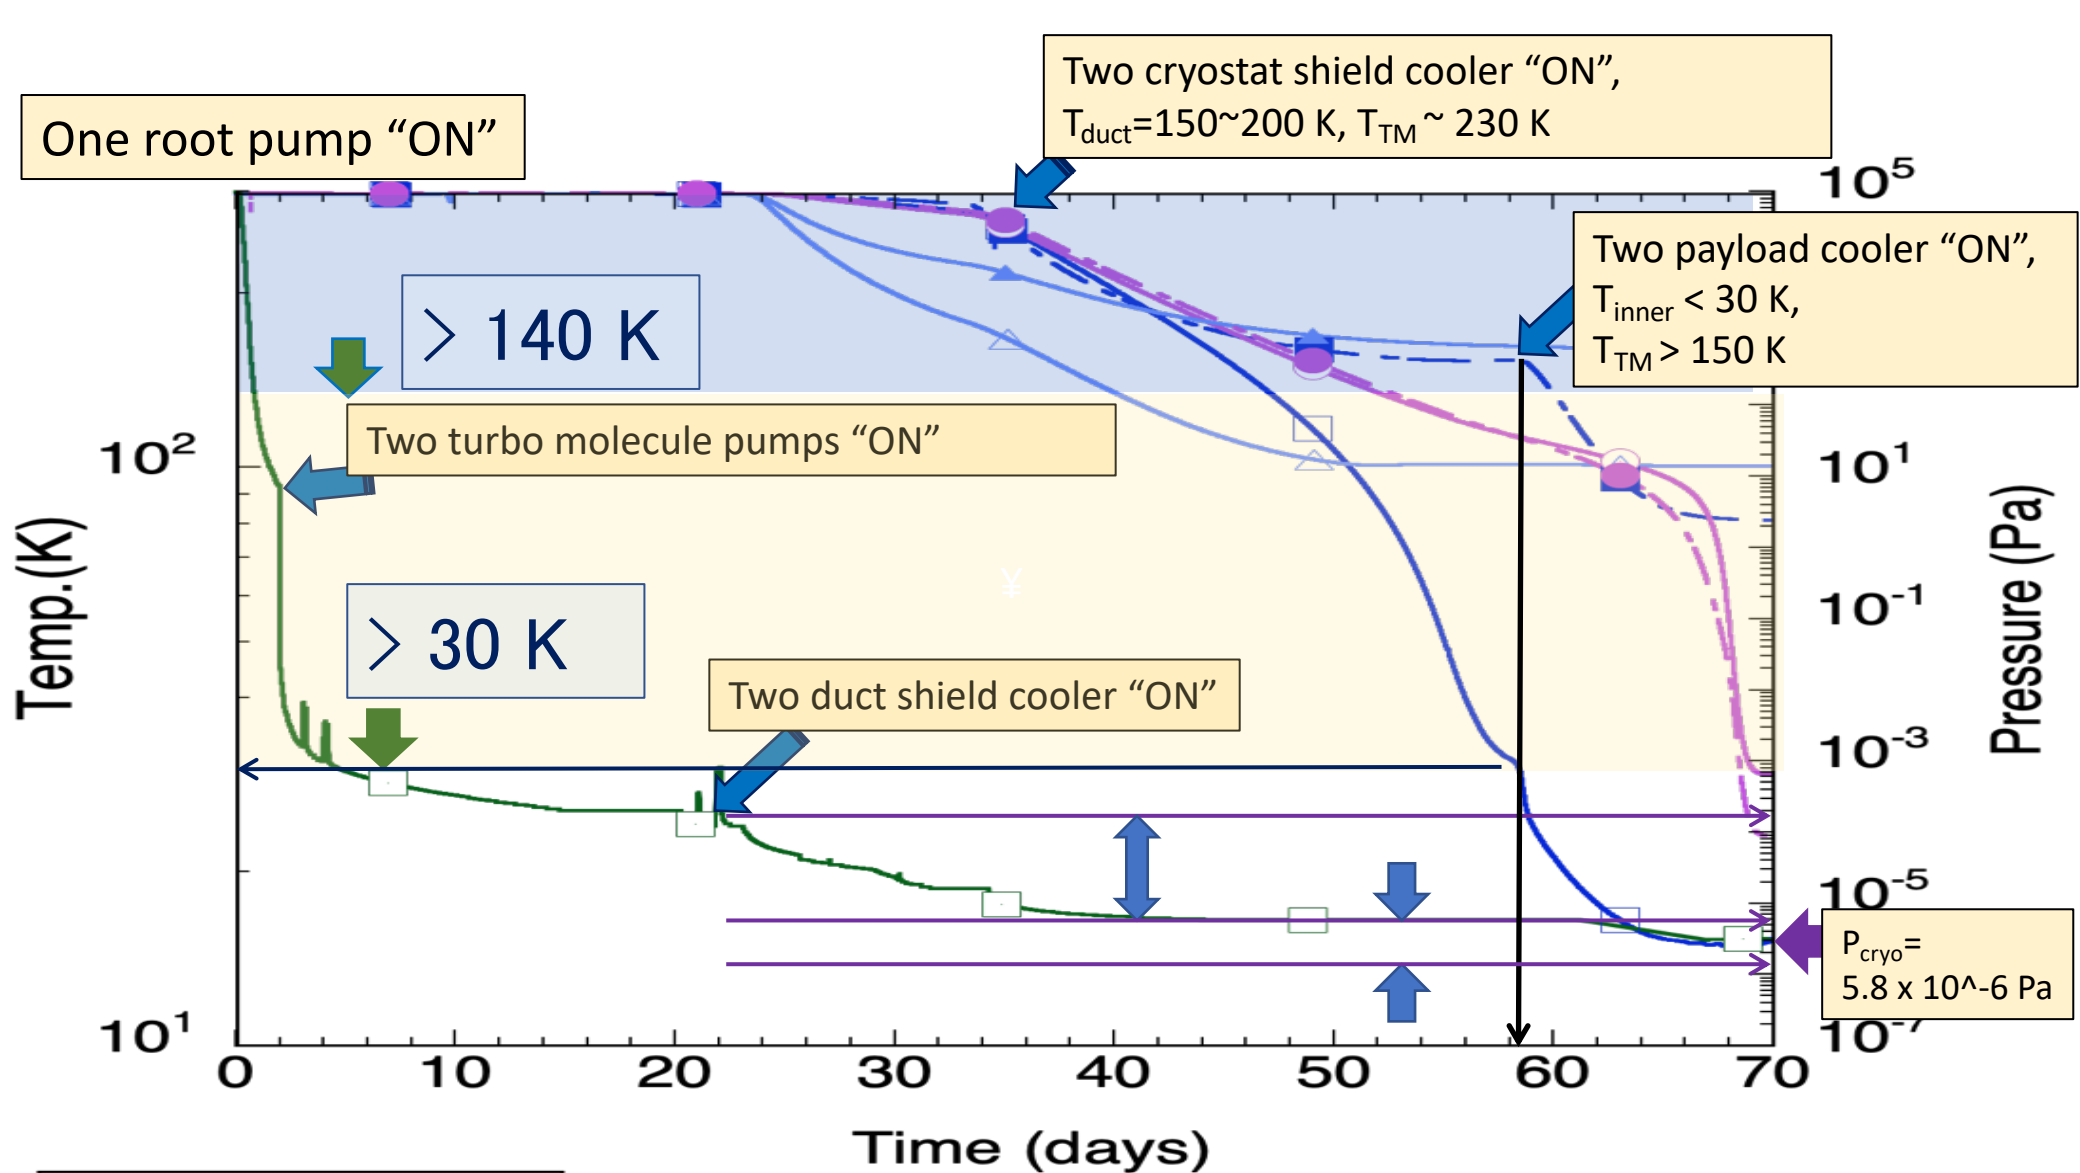

Temperature dependence of internal pressure

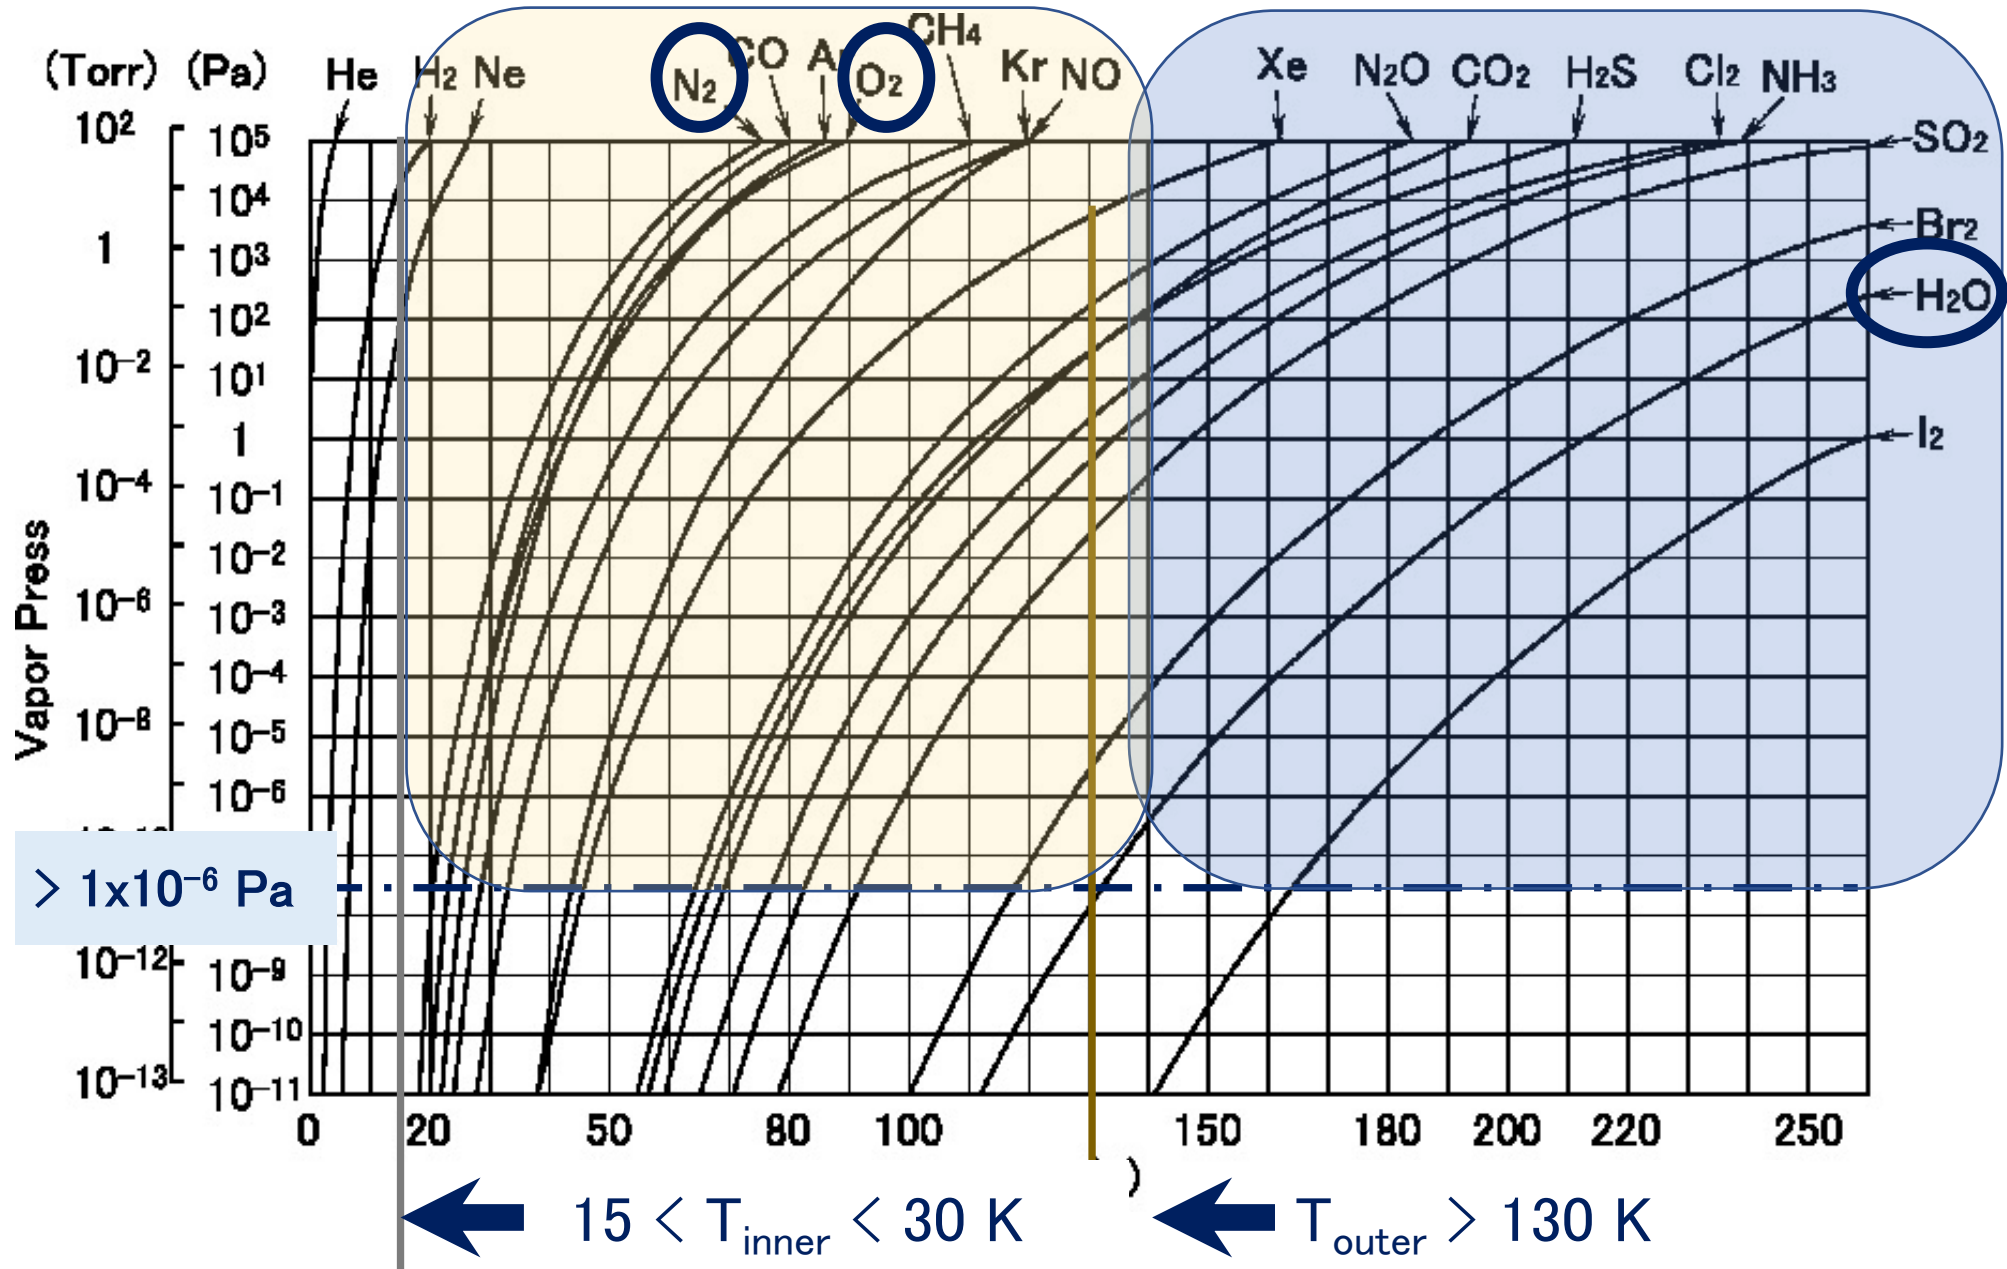


Trap O<sub>2</sub> & N<sub>2</sub> by inner shield

Trap H<sub>2</sub>O by duct & outer shields

# Defrost heater layout

A small heater was attached on IM for defrost of mirror surface.

Two calibration heaters were equipped with the top of inner radiation shield.

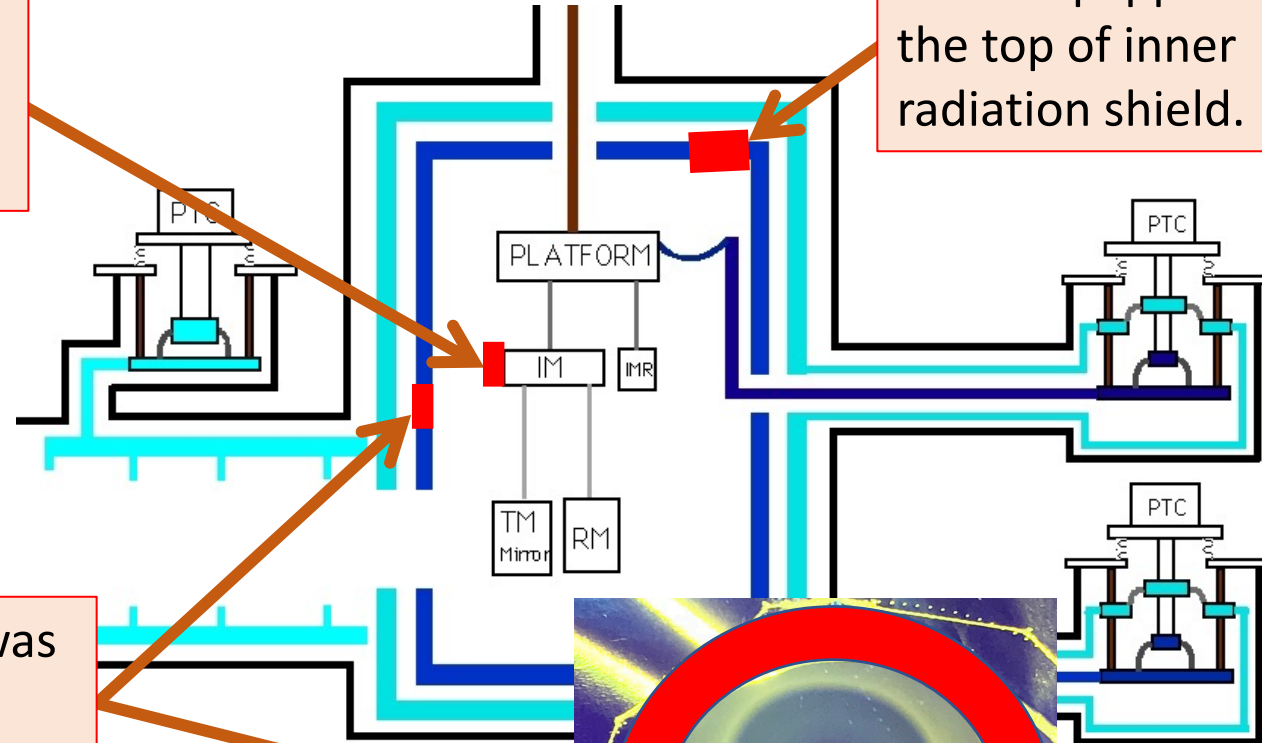

A defrost heater was attached on view port.

- Three kinds of heaters for defrosting were installed in KAGRA cryostat.






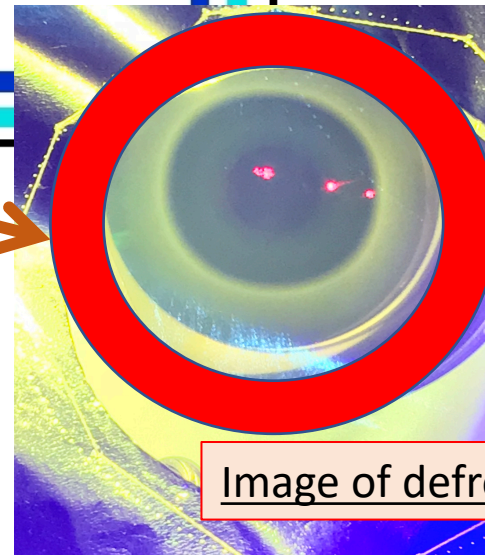


Image of defrost heater

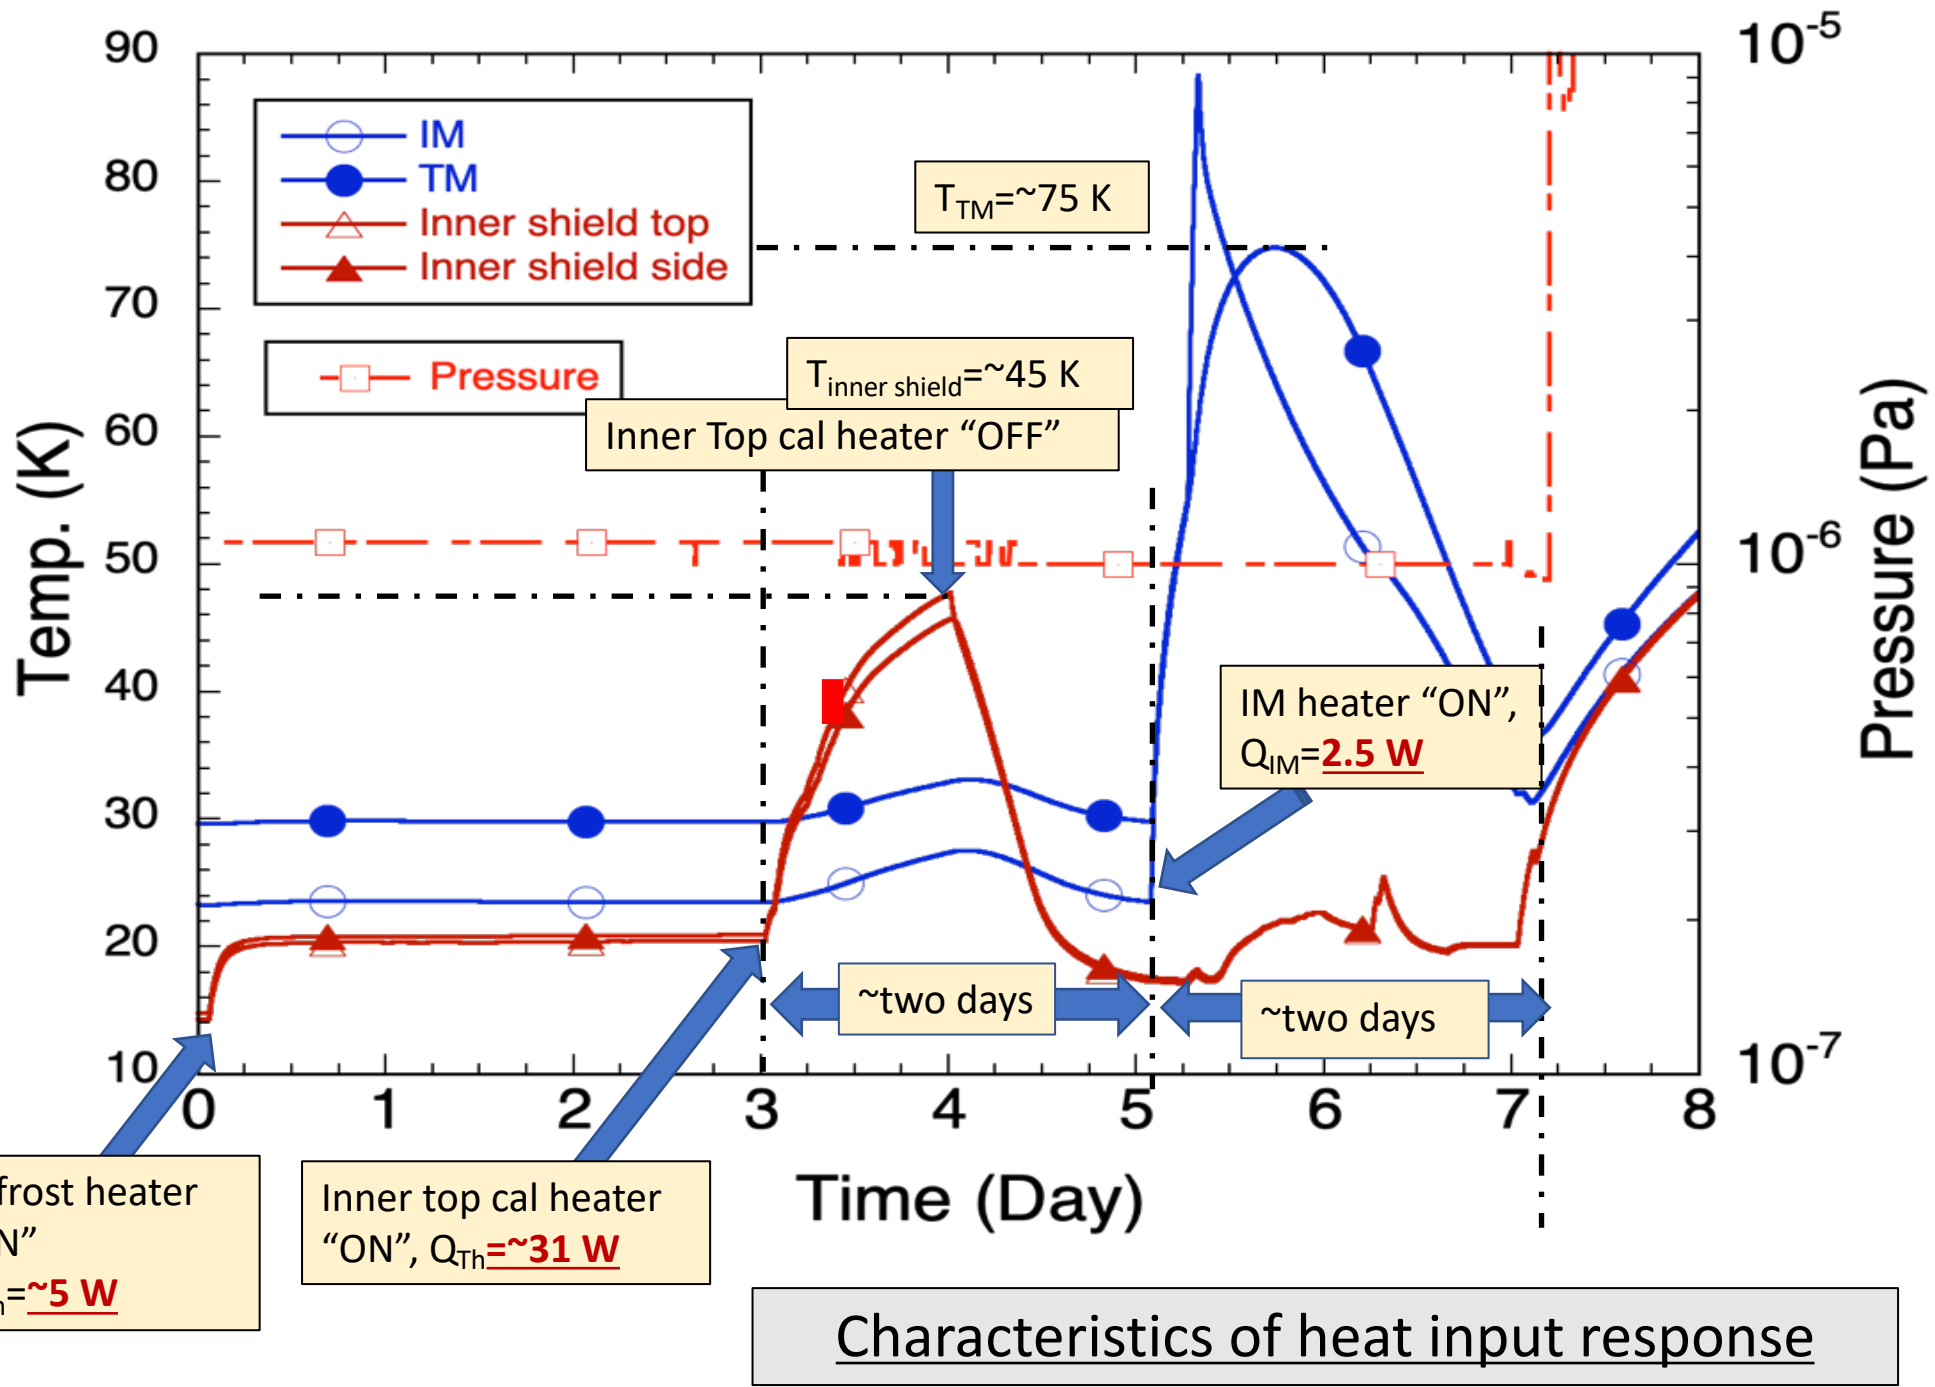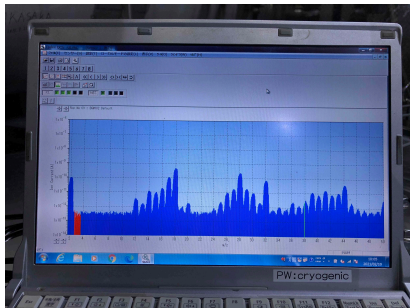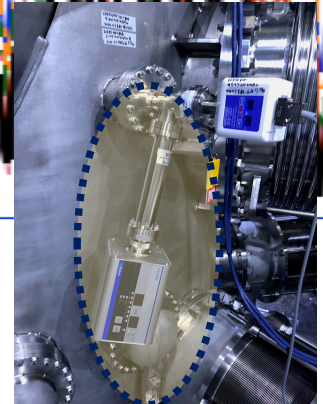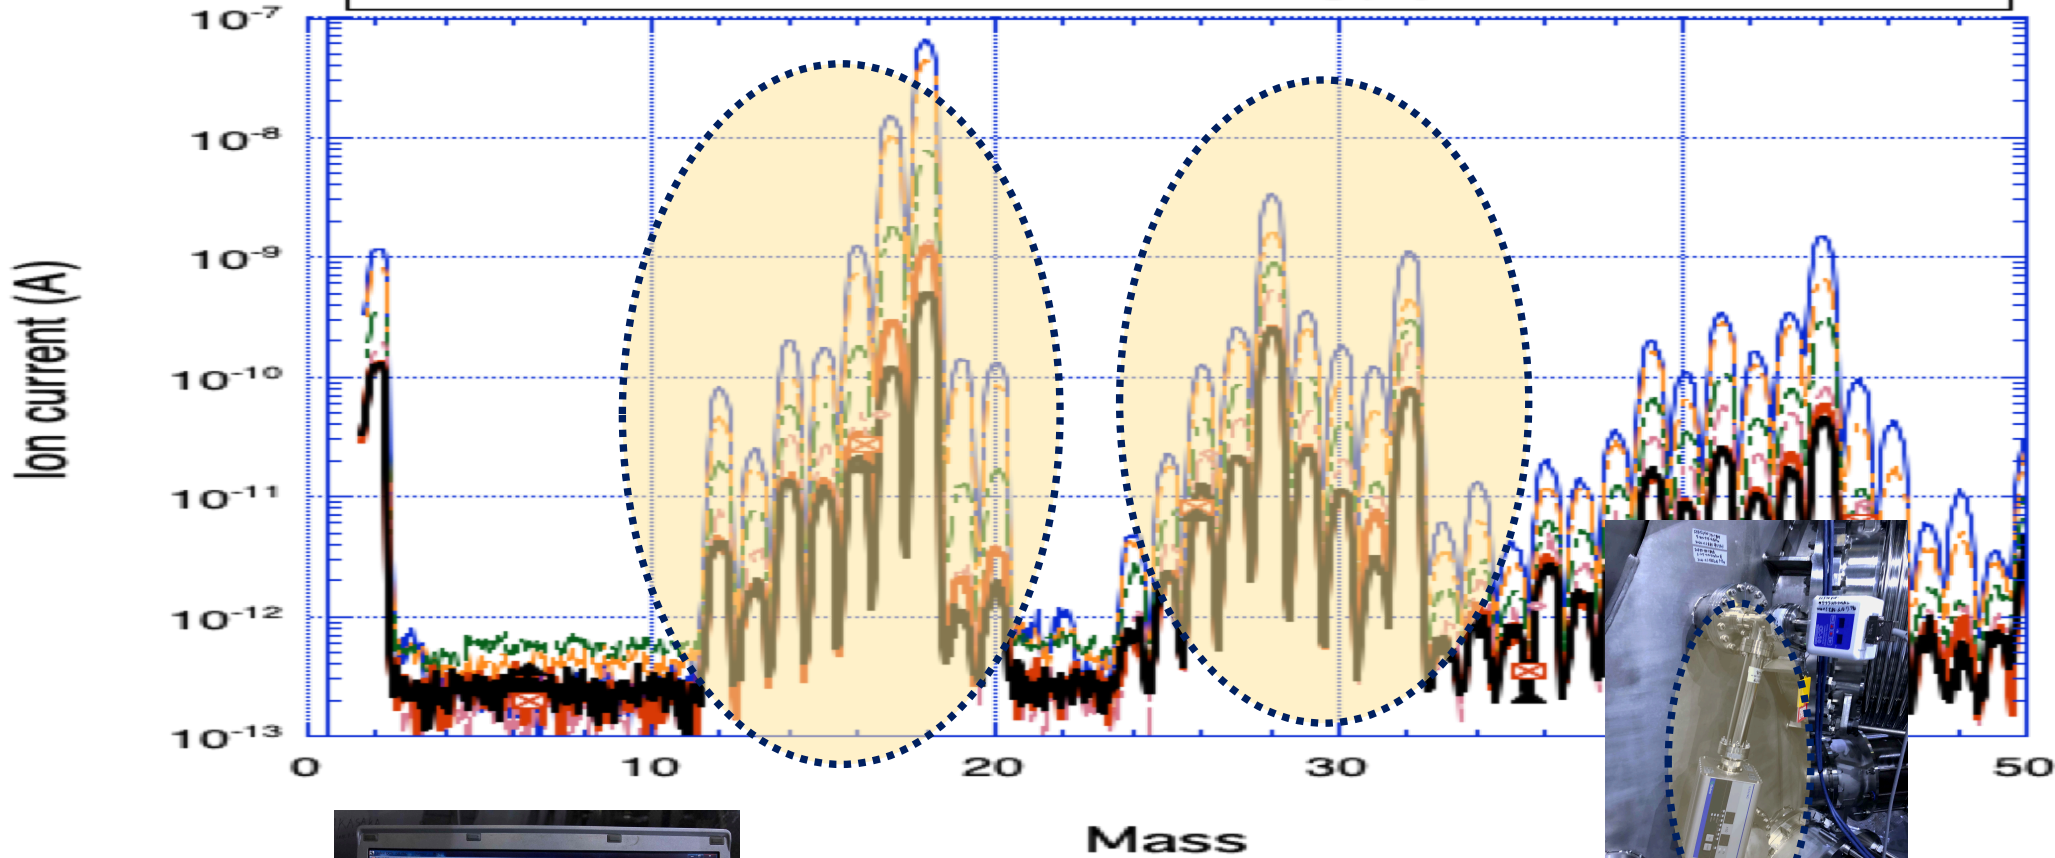


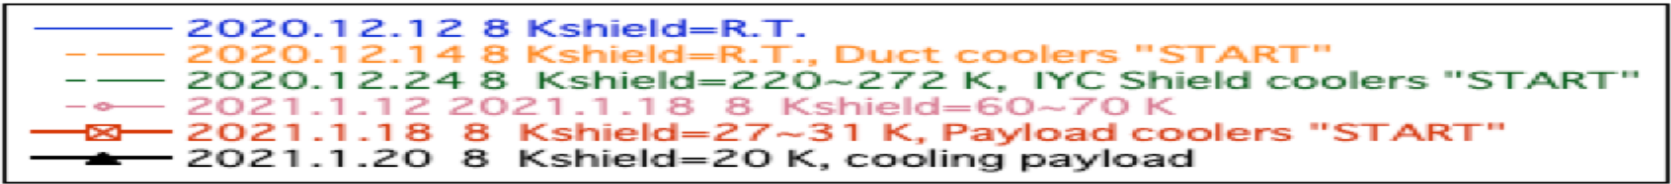

Temperature dependence of Q-mass

H<sub>2</sub>O

N<sub>2</sub>

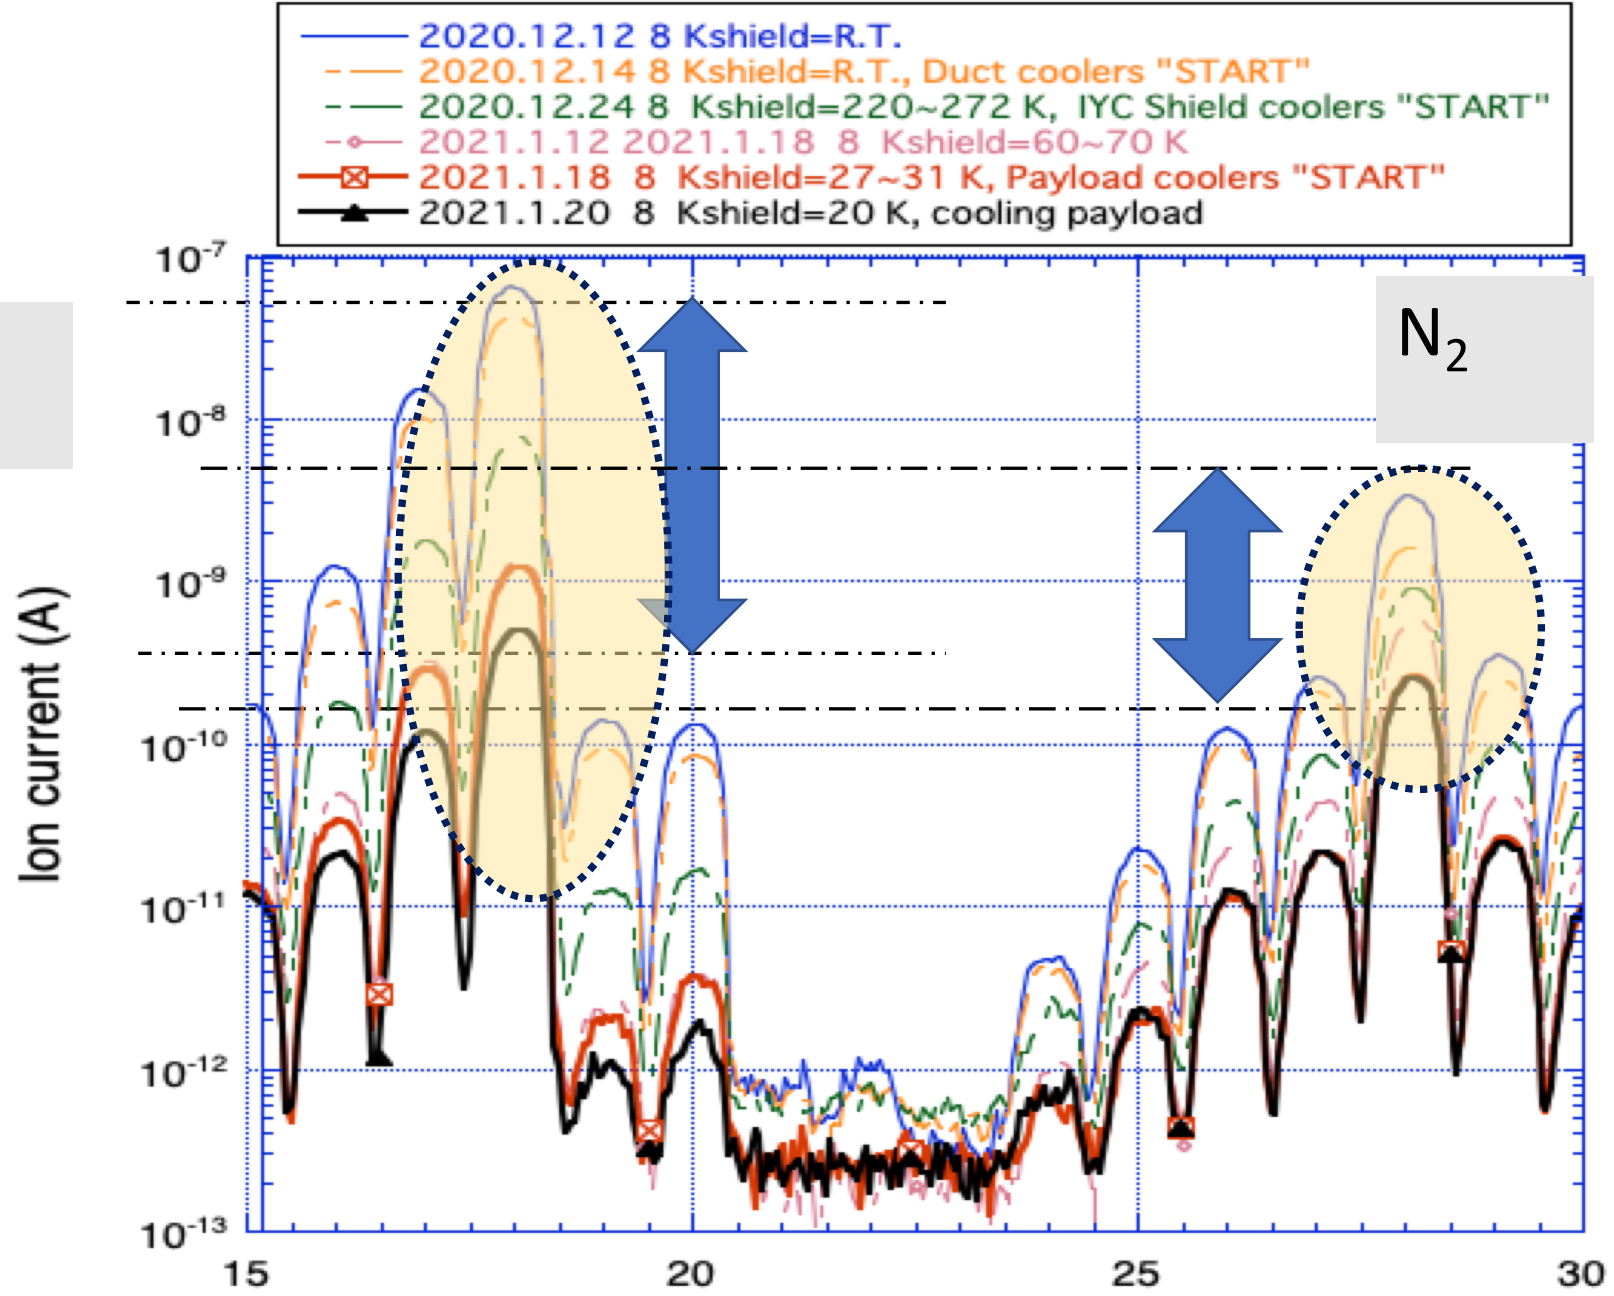

Temperature dependence of Q-mass

Mass


# Summaries

- Frost on the surface of view ports were not appeared during this experiment!
- Following items were confirmed in this experiment;
  - ✓ Frost on the view ports are not appeared by proposed cooling scenario.
  - ✓ Calibration heaters on the surface of inner radiation shield well worked as defrost heater for view ports on the surface of inner radiation shield up to  $\sim 50$  K. It will take **2 days** for defrosting for surface of the view ports.
  - ✓ Heater on the IM well worked as defrost heater for mirror on the up to  $\sim 70$  K. It will take **2 days** for defrosting for surface of mirror.
  - ✓ Partial pressure measurement of residual gas at each temperature was performed.

# Appendix




# Overview of KAGRA Cryogenics system

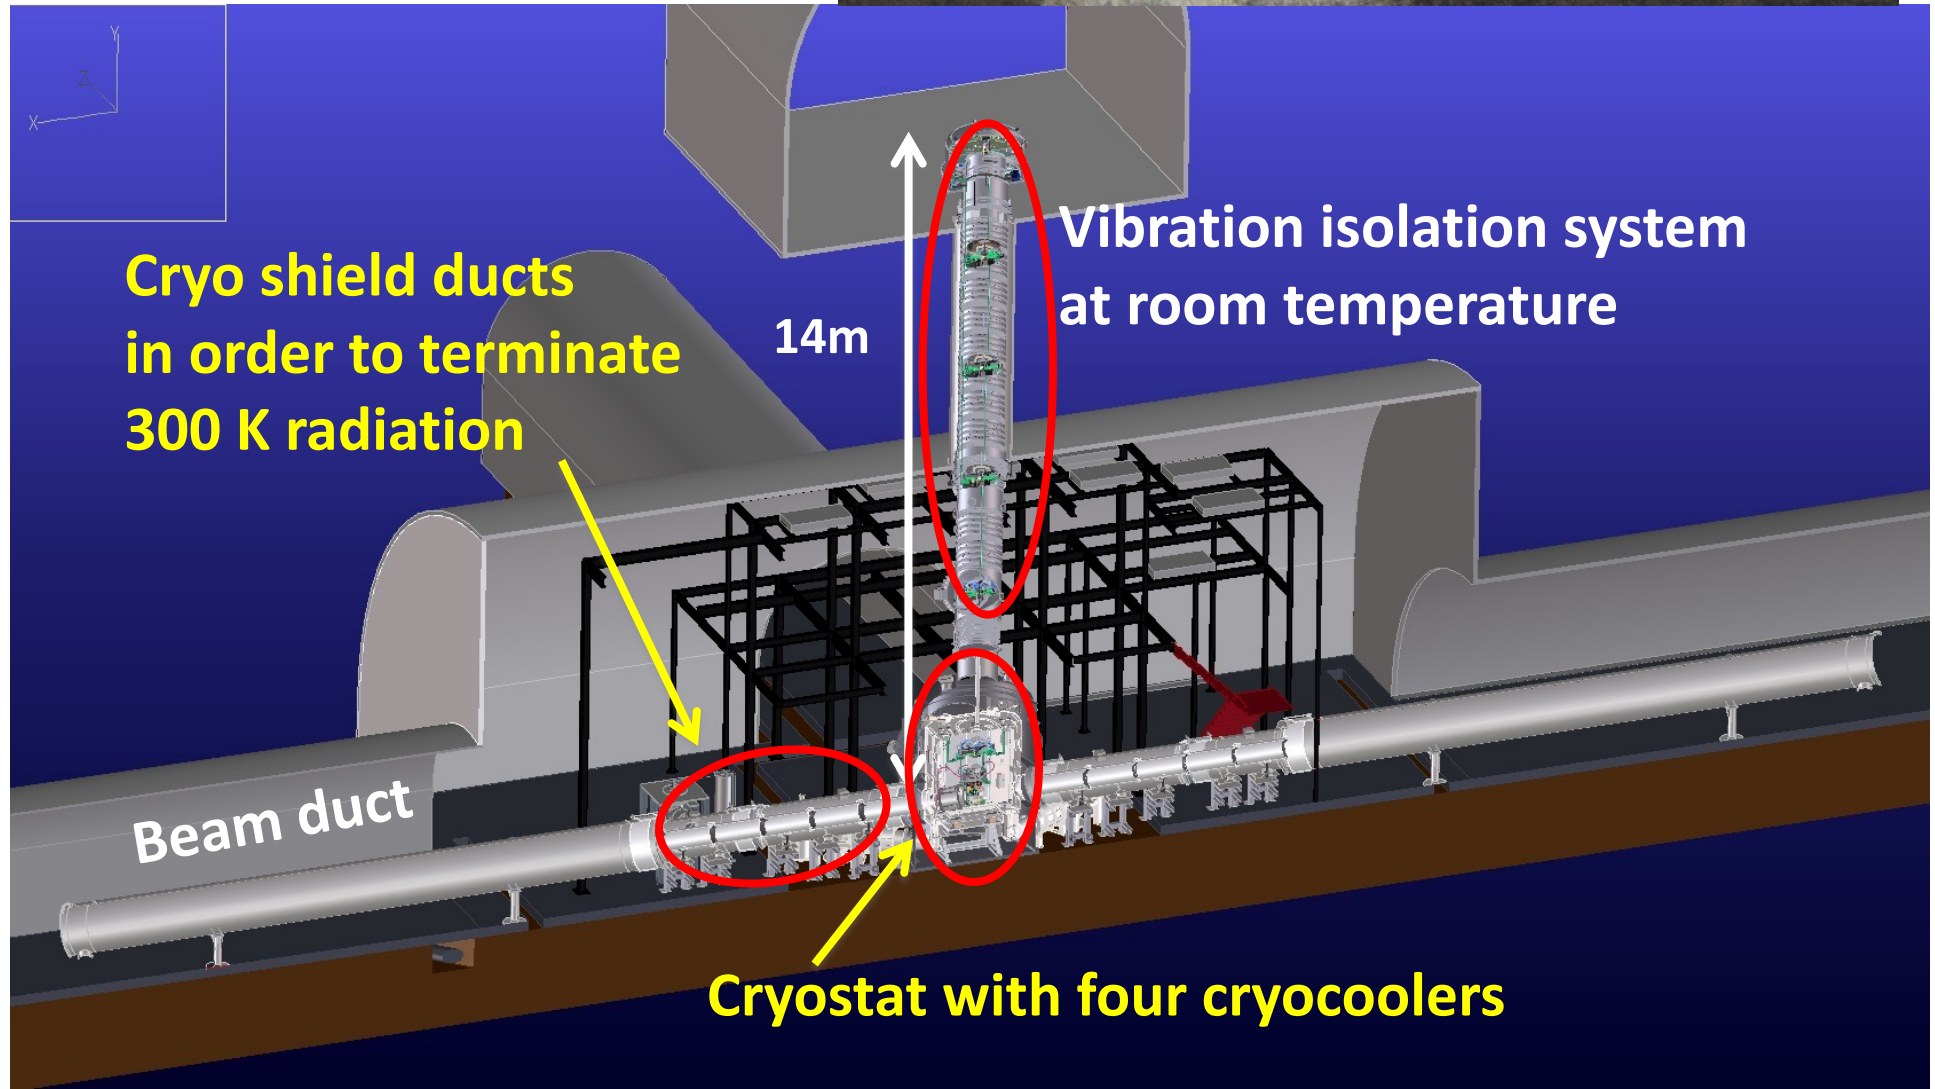


# Structure of KAGRA Cryostat

Stainless steel  $t=20\text{mm}$   
Diameter 2.4 m  
Height  $\sim 4.3\text{ m}$   
 $M \sim 12\text{ ton}$   
Cold Mass:  
8K shield  $\sim 455\text{ kg}$   
80 K shield  $\sim 590\text{ kg}$

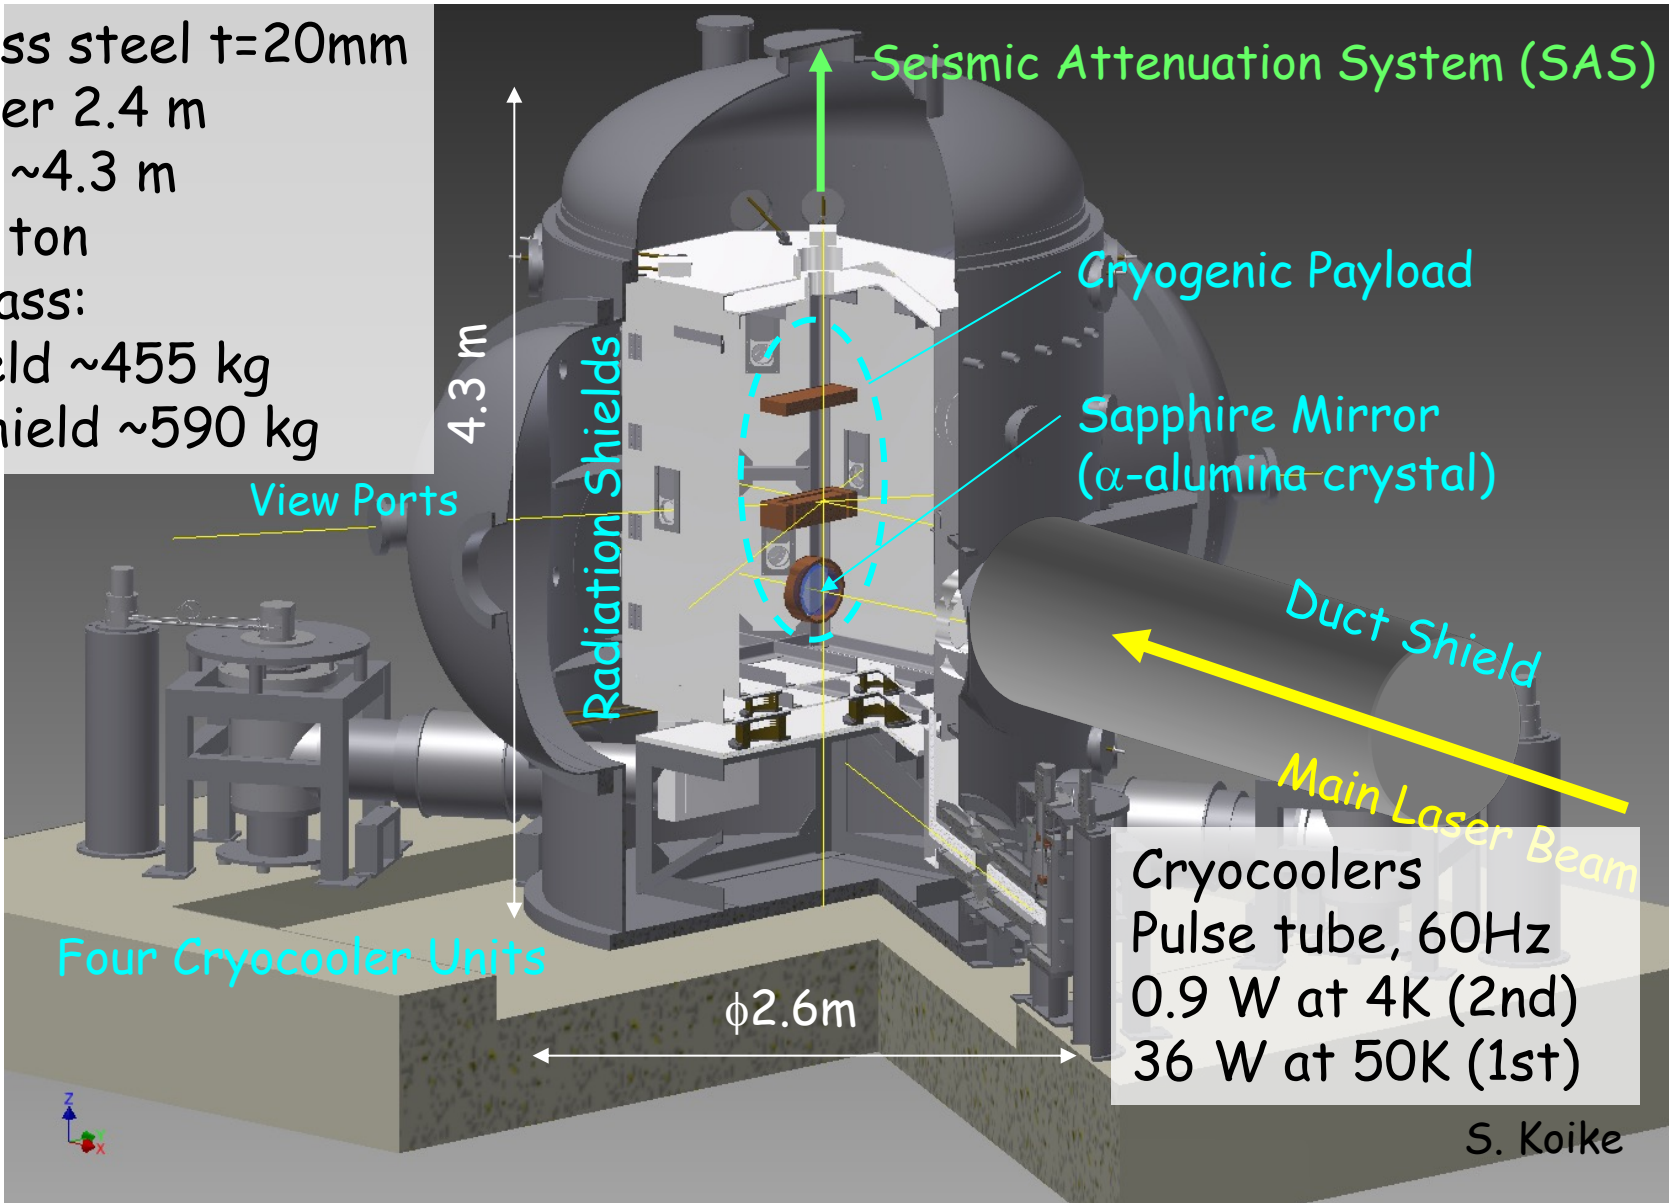


Cryocoolers  
Pulse tube, 60Hz  
0.9 W at 4K (2nd)  
36 W at 50K (1st)

S. Koike

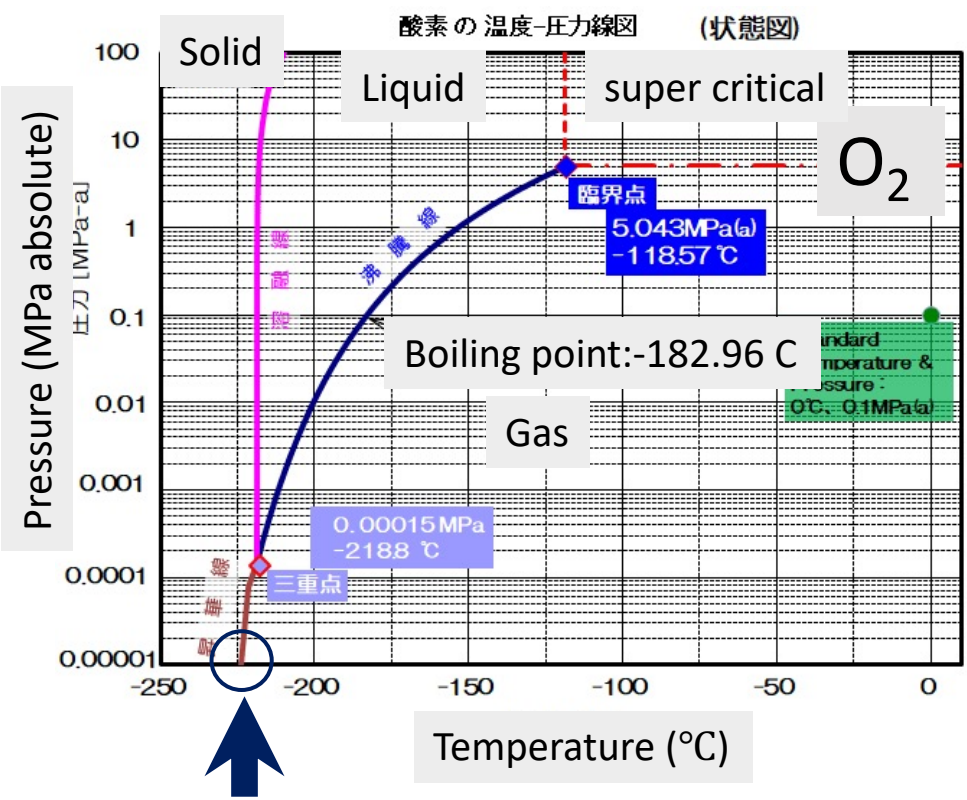


$1 \times 10^{-5} \text{ Pa} \rightarrow \sim -225 \text{ }^\circ\text{C} (\sim 48 \text{ K})$

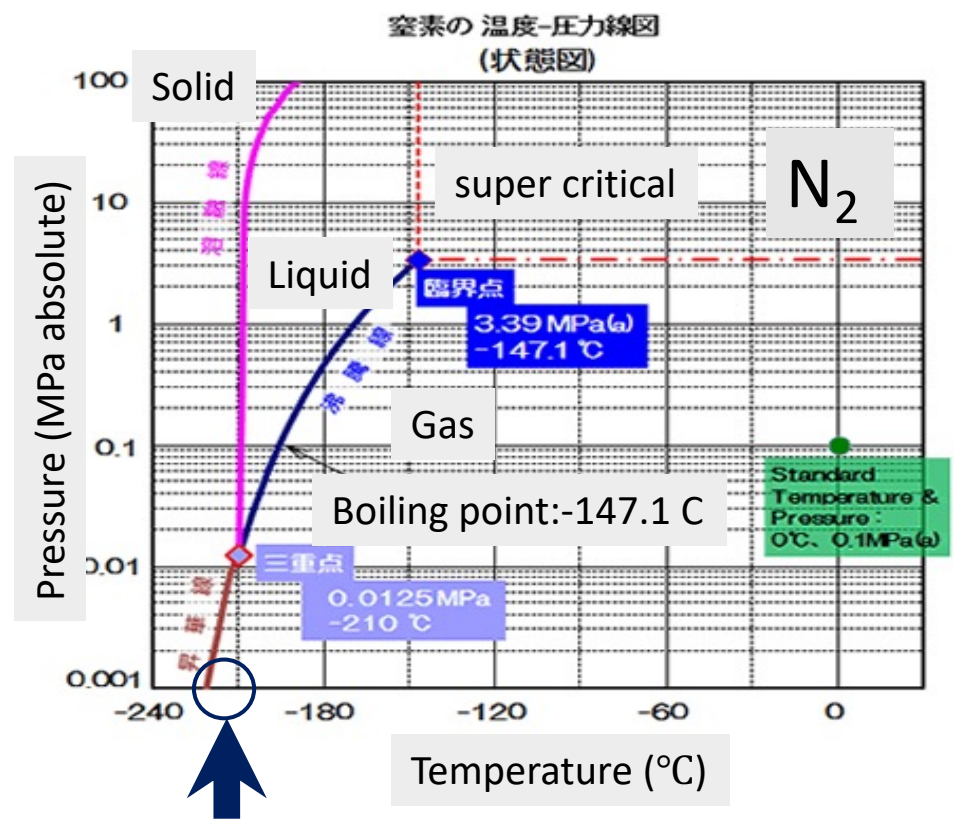

$1 \times 10^{-3} \text{ Pa} \rightarrow \sim -220 \text{ }^\circ\text{C} (\sim 53 \text{ K})$

State diagrams of O2 and N2

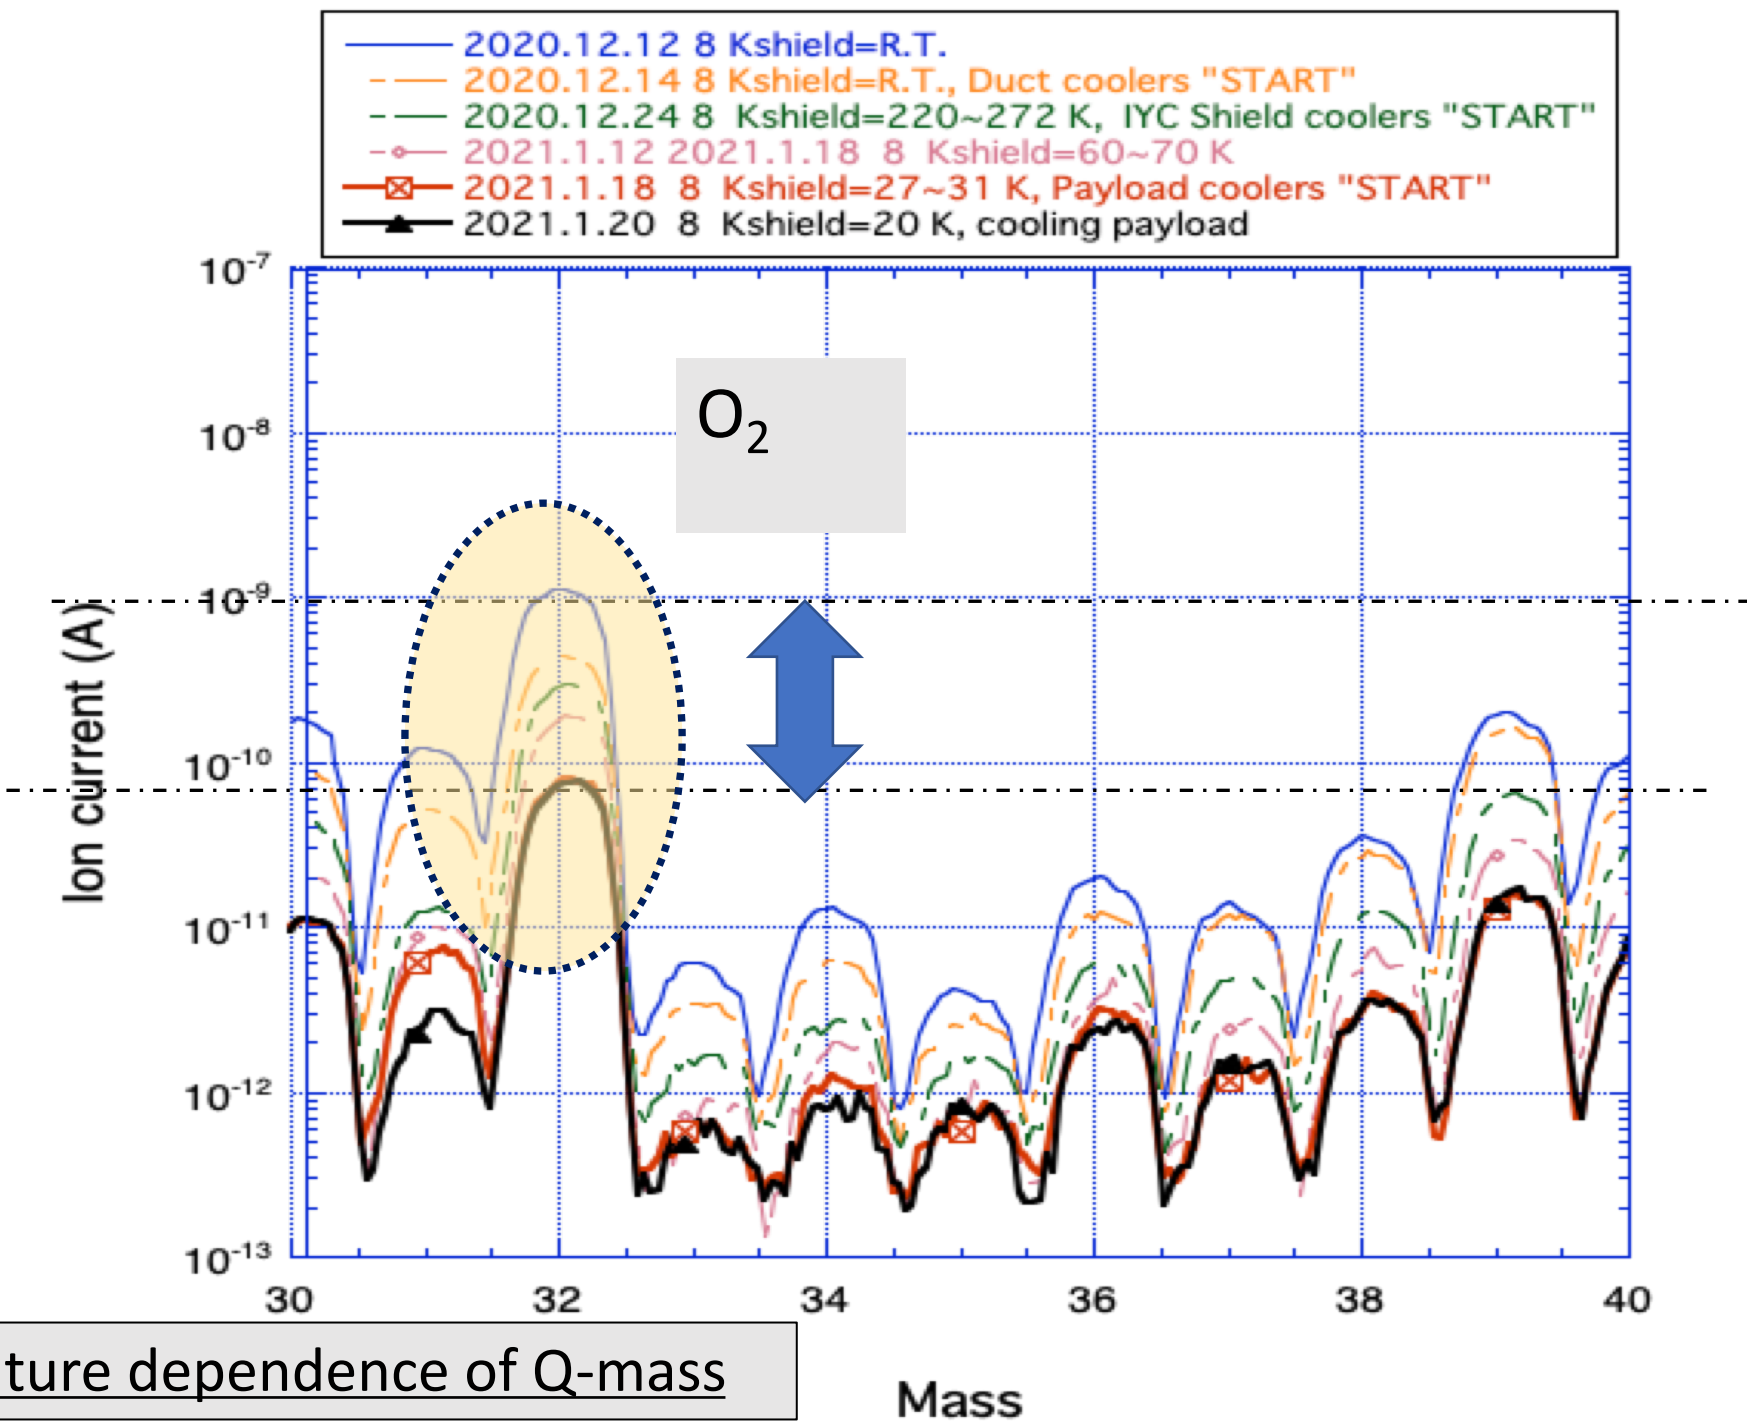

Temperature dependence of Q-mass